

Tria™ Soft Ureteral Stent Calcium and Magnesium Urine Salt Accumulation:

Evaluation of Novel Anti-Adherence
Materials on Tria Soft and Coloplast
Imajin® Ureteral Stents Using the
BEST™ Method

Testing conducted by Innovotech Inc.

A pioneer in antimicrobial and anti-encrustation testing
for coated medical devices.

Introduction and Purpose

Despite continued advances in ureteral stent design and materials, the problem of minimizing the encrustation of biomaterials in the urinary tract remains a challenge. It is well documented that both major and minor stent encrustations can lead to stent blockage and adverse effects, including flank pain, infection, irritative urinary symptoms, hydronephrosis, etc.¹ Encrusted stents can also be difficult to remove and may require additional, often complicated, surgical procedures.^{1,2} The cause and rate of encrustation is multifactorial and can include factors such as body chemistry and medical condition of the patient, stent in-dwell time, and surface material or properties of the stent.²⁻⁴

The Tria Ureteral Stent is designed with a unique tri-layer design, including a proprietary PercuShield™ technology on both the outer and inner stent surfaces that minimizes the adherence of calcium and magnesium salts. The PercuShield technology is designed with an inert, non-polar copolymer material composition, which has a low surface energy. Consequently, the surface is less reactive to aqueous solutions, and less compatible with ionic materials such as urine calcium and magnesium salts,⁵ which is one of many factors impacting encrustation.^{4,6}

The purpose of this paper is to summarize the findings of a laboratory study evaluating the ability of Tria Soft Ureteral Stent's inner and outer surface layers to minimize the accumulation of calcium and magnesium urine salt deposits on the stent surface compared to uncoated Coloplast Imajin™ Silicone Stent.

Since the presence of a urinary tract infection may also correlate with a higher degree of distal coil encrustation,⁷ the adherence of calcium and magnesium salts to the stent surface was analyzed both in the presence and in the absence of bacteria.

Materials and Methods


Testing was performed by Innovotech, Inc. using the in-vitro BEST™ (Biofilm Eradication Surface Testing) platform to evaluate calcium and magnesium salt accumulation of the ureteral stents.⁵

A total of 30 samples from each ureteral stent family (Tria Soft and uncoated Coloplast Imajin Silicone), cut into 3.5cm pieces, were tested in a sterile Artificial Urine Model and a Bacterial Infection Model (n=15 in each model). All samples tested contained side holes, allowing the urine to flow in and out of the side holes freely.

Units tested in the "Sterile Urine" group were soaked in artificial urine, filtrated through 0.2 µm filter units and stored at 4°C until required. Before use, a sterility check was performed. Units tested in the "Bacterial Infection Model" group were soaked in sterile artificial urine with a *Proteus mirabilis* spike. *Proteus mirabilis* was used as the microbial challenge in the Bacterial Infection Model due to its known urease production and involvement in struvite formation.⁸ Artificial urine was replaced every 48 hours. Units in both models were secured to pegs in the BEST™ 12 well plate, ensuring they were in a "U" shape, with a simulated 0.5 ml/min physiological flow rate; incubated at 37±2°C for 2 weeks.

Upon completion of the 2-week exposure, salt crystals were disrupted by sonicating in nitric acid solution for 30 min and left for 24 hours, and solutions were analyzed for calcium and magnesium content by atomic absorption spectroscopy (AAS).


Cross-section view of Tria™ Stent

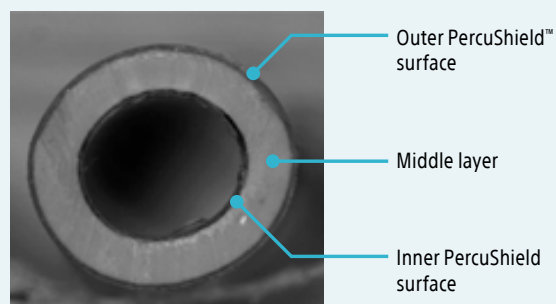

Results

After 2 weeks of soaking (artificial urine was changed every 48 hours), the recovered magnesium (Mg) and calcium (Ca) salt accumulation in nitric acid was measured. In the "Bacterial Infection Model" the adhered microbial biomass was recovered first, then the recovered Mg and Ca salt accumulation in nitric acid was measured. For both conditions, the mean material (mg/cm²), as well as comparative difference calculated as [(Tria™ Soft Stent – Competitor Stent) / Competitor Stent] * 100 was analyzed.


Sterile Artificial Urine Study

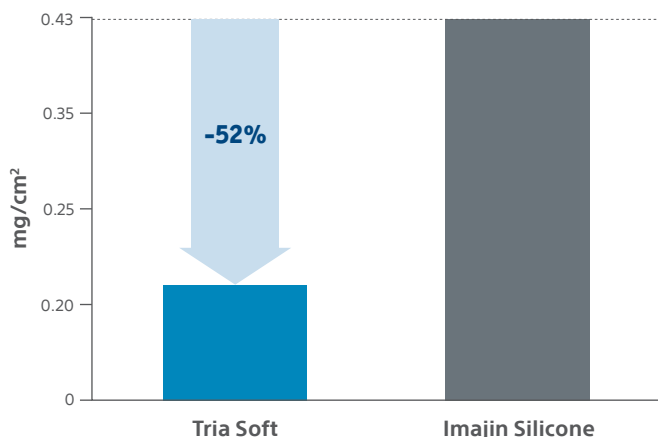

The Tria Soft Stent reduced the combined Ca and Mg Urine Salt Accumulation by 52% compared to the Coloplast Imajin Silicone Stent in the sterile urine model. The mean difference of salt crystal material was a statistically significant reduction.

Device	Mean Material (mg/cm ²)	St. Dev	P-Value*	Difference (mg/cm ²)	% Difference
Tria Soft	0.2090	0.0366	<0.001	-0.2231	-52%
Imajin Silicone	0.4322	0.0494			

Proteus Spiked Artificial Urine Study

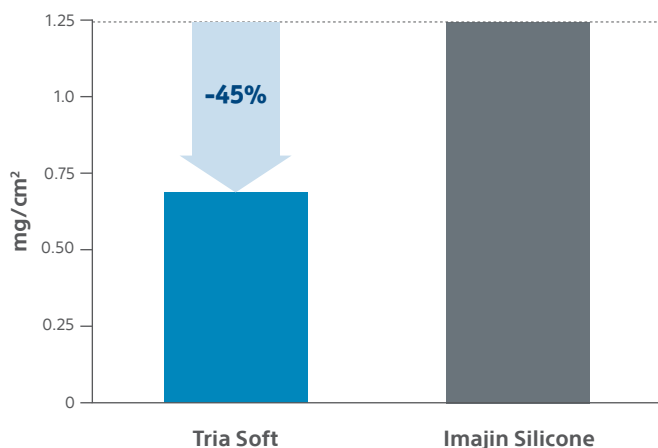

The Tria Soft Stent reduced the combined Ca and Mg Urine Salt Accumulation by 45% compared to the Coloplast Imajin Silicone Stent in the bacterial infection urine model. The mean salt crystal material was a statistically significant reduction.

Device	Mean Material (mg/cm ²)	St. Dev	P-Value*	Difference (mg/cm ²)	% Difference
Tria Soft	0.6808	0.0788	<0.001	-0.5689	-45%
Imajin Silicone	1.2497	0.0872			

* For each condition, the difference between the Tria Stent and the Coloplast Imajin Silicone Stent on mean amount of salt crystal material was assessed at the 0.05 level of significance using a (one-sided) two-sample t test.

Conclusion

In conclusion, the data collected and analyzed as part of this study provide evidence that Tria™ Soft Stent's unique tri-layer design, with the PercuShield™ technology on both the outer and inner surfaces of the stent, significantly reduced the combined accumulation of magnesium and calcium deposits when compared to the uncoated Coloplast Imajin™ Silicone Stent both in the presence and in the absence of bacteria (*Proteus mirabilis*).⁵

1. Arenas JL, Shen JK, Keheila M, et al. Kidney, ureter, and bladder (KUB): A novel grading system for encrusted ureteral stents. *Urology*. 2016 Nov;97:51-5.
2. Bultitude MF, Tiptaft RC, Glass JM, et al. Management of encrusted ureteral stents impacted in upper tract. *Urology*. 2003 Oct;62(4):622-6.
3. Elwood CN, Lo J, Chou E, et al. Understanding urinary conditioning film components on ureteral stents: profiling protein components and evaluating their role in bacterial colonization. *Biofouling*. 2013;29(9):1115-22.
4. Vanderbrink BA, Rastinehad AR, Ost MC, et al. Encrusted urinary stents: Evaluation and endourologic management. *J Endourol*. 2008 May;22(5):905-12.
5. Data on file with Boston Scientific.
6. Bruce AW, Sira SS, Clark AF, et al. The problem of catheter encrustation. *Can Med Assoc J*. 1974 Aug 3;111(3):238-9 passim.
7. Sighinolfi MC, Sighinolfi GP, Galli E, et al. Chemical and mineralogical analysis of ureteral stent encrustation and associated risk factors. *Urology*. 2015 Oct;86(4):703-6.
8. Brooks T, Keevil CW. A simple artificial urine for the growth of urinary pathogens. *Lett Appl Microbiol*. 1997 Mar;24(3):203-6.

The testing was performed by or on behalf of Boston Scientific. Data on file.

Bench test results may not necessarily be indicative of clinical performance.

CAUTION: US Federal law restricts this device to sale by or on the order of a physician.

CAUTION: The law restricts these devices to sale by or on the order of a physician. Indications, contraindications, warnings and instructions for use can be found in the product labeling supplied with each device. Products shown for INFORMATION purposes only and may not be approved or for sale in certain countries. This material not intended for use in France.

All trademarks are the property of their respective owners.

© 2021 Boston Scientific Corporation or its affiliates. All rights reserved. URO-1022005-AA JUN 2021