


Laser Cut Self-Expanding Metal Stent

The Epic Biliary Endoscopic Stent System was developed to complement our best-in-class braided metal stent portfolio. The Epic Biliary Endoscopic Stent System is indicated for palliation of malignant neoplasms in the biliary tree. It may be used to palliate strictures caused by unresectable Bile Duct Cholangiocarcinoma. The Epic Biliary Stent was developed for physicians who prefer a laser cut stent.

Epic Biliary Endoscopic Stent System

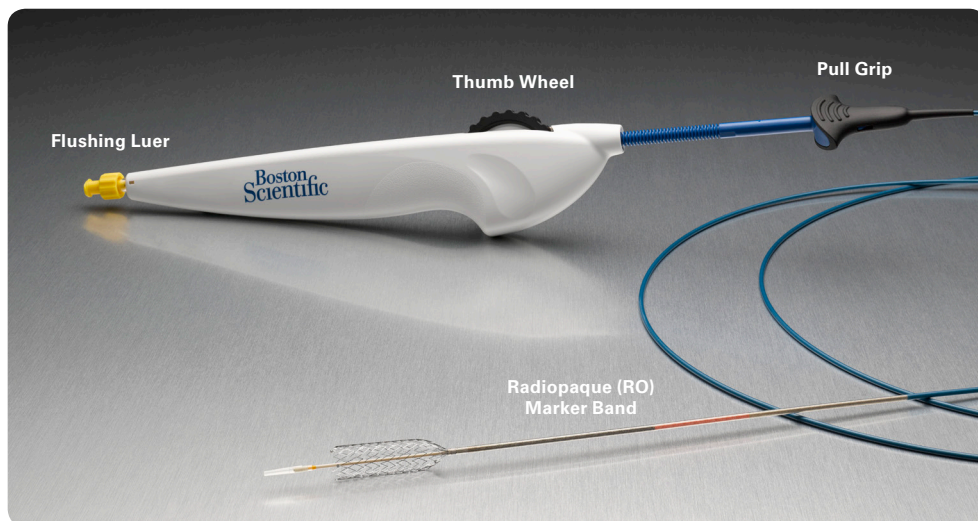

Dual Deployment Method Delivery System

Thumb wheel deployment with auditory indicators and tactile feedback for ease of placement and control, or the optional pull grip.

Optimization of Laser Cut Design

Minimal Foreshortening

Aid in placement

Low Profile 6Fr Catheter

Designed to help place the stent across tighter strictures

Up to 100mm Stent Length


May help to reduce the need for placement of additional stents

Tantalum Radiopaque Markers at the Distal and Proximal End of the Stent

Enhanced fluoroscopic visualization to aid in deployment precision

220cm Catheter

Compatible with duodenoscopes for standard ERCP procedures and balloon enteroscopy-assisted ERCP scopes

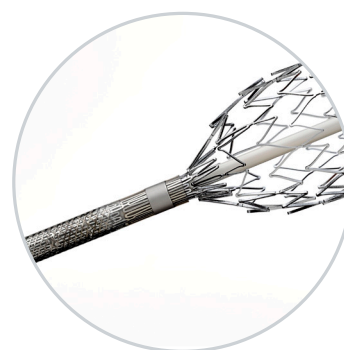

Reimbursement Codes

Placement of a Biliary Metal Stent

CPT Code	Code Description
43274	Endoscopic retrograde cholangiopancreatography (ERCP); with placement of endoscopic stent into biliary or pancreatic duct, including pre- and post- dilation and guidewire passage, when performed, including sphincterotomy, when performed, each stent
43275	Endoscopic retrograde cholangiopancreatography (ERCP); with removal of foreign body(s) or stent(s) from biliary/pancreatic duct(s)
43276	Endoscopic retrograde cholangiopancreatography (ERCP); with removal and exchange of stent(s), biliary or pancreatic duct, including pre- and post- dilation and guidewire passage, when performed, including sphincterotomy, when performed, each stent exchanged
C-Code	Code Description
C1876	Stent- non-coated/non-covered, with delivery system

Ordering Information

Product Code	Description	Stent Diameter (mm)	Stent Length (mm)	Catheter Diameter (Fr)	Guidewire Diameter (in)	Catheter Working Length (cm)	Pricing
M00572230	Epic Biliary Stent	6	40	6	0.035	220	<input type="text"/>
M00572240	Epic Biliary Stent	6	60	6	0.035	220	<input type="text"/>
M00572250	Epic Biliary Stent	6	80	6	0.035	220	<input type="text"/>
M00572260	Epic Biliary Stent	6	100	6	0.035	220	<input type="text"/>
M00572270	Epic Biliary Stent	8	40	6	0.035	220	<input type="text"/>
M00572280	Epic Biliary Stent	8	60	6	0.035	220	<input type="text"/>
M00572290	Epic Biliary Stent	8	80	6	0.035	220	<input type="text"/>
M00572300	Epic Biliary Stent	8	100	6	0.035	220	<input type="text"/>
M00572310	Epic Biliary Stent	10	40	6	0.035	220	<input type="text"/>
M00572320	Epic Biliary Stent	10	60	6	0.035	220	<input type="text"/>
M00572330	Epic Biliary Stent	10	80	6	0.035	220	<input type="text"/>
M00572340	Epic Biliary Stent	10	100	6	0.035	220	<input type="text"/>

Boston Scientific Contact Information

Name:

Phone Number:

Title:

E-mail:

For ordering information, please contact your Boston Scientific Sales Representative or visit www.bostonscientific.com

CPT Copyright 2016 American Medical Association. All rights reserved. CPT is a registered trademark of the American Medical Association. Applicable FARS/DFARS Restrictions Apply to Government Use. Fee schedules, relative value units, conversion factors and/or related components are not assigned by the AMA, are not part of CPT, and the AMA is not recommending their use. The AMA does not directly or indirectly practice medicine or dispense medical services. The AMA assumes no liability for data contained or not contained herein.

Health economic and reimbursement information provided by Boston Scientific Corporation is gathered from third-party sources and is subject to change without notice as a result of complex and frequently changing laws, regulations, rules and policies. This information is presented for illustrative purposes only and does not constitute reimbursement or legal advice. Boston Scientific encourages providers to submit accurate and appropriate claims for services. It is always the provider's responsibility to determine medical necessity, the proper site for delivery of any services and to submit appropriate codes, charges, and modifiers for services that are rendered. Boston Scientific recommends that you consult with your payers, reimbursement specialists and/or legal counsel regarding coding, coverage and reimbursement matters. Boston Scientific does not promote the use of its products outside their FDA-approved label.

Caution: U.S. Federal law restricts this device to sale by or on the order of a physician.

CAUTION: The law restricts these devices to sale by or on the order of a physician. Indications, contraindications, warnings and instructions for use can be found in the product labelling supplied with each device. Information for use only in countries with applicable health authority registrations. Material not intended for use in France.

Warning: The safety and effectiveness of this device for use in the vascular system have not been established.

Warning: Once the stent is partially deployed, it cannot be "recaptured" or "resheathed" using the stent delivery system.

**Boston
Scientific**
Advancing science for life™

Boston Scientific Corporation
300 Boston Scientific Way
Marlborough, MA 01752-1234
www.bostonscientific.com/gastro
www.EndoSuite.com

©2017 Boston Scientific Corporation
or its affiliates. All rights reserved.

ENDO-501004-AA October 2017