


Prevalence of Procedures

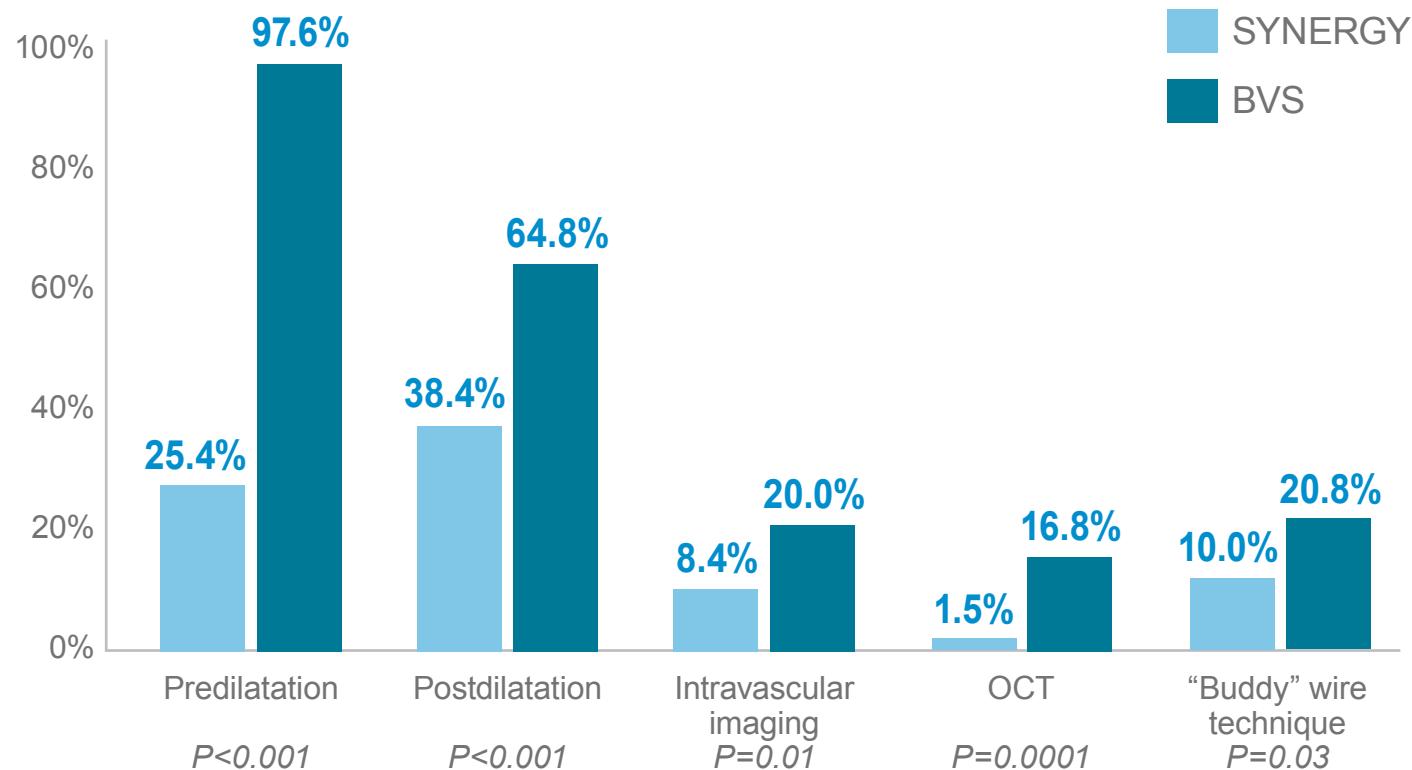

Procedures with BVS

	SYNERGY	BVS	P-value
Fluoroscopy time (min)	39 ± 21	46 ± 20	0.01
Median dose-area product (mGy cm ²)	57698	69432	0.02
Contrast volume (ml)	235 ± 80	260 ± 85	0.03
Postprocedure Troponin I (ng/ml)	1.16 ± 2.6	2.62 ± 6	0.02
Increase in Troponin I (ng/ml)	1.14 ± 2.5	2.6 ± 6.1	0.02