

# SYNERGY™


Everolimus-Eluting Platinum Chromium  
Coronary Stent System

## Leading in Complex Patients

Short DAPT with the SYNERGY BP Stent

The SYNERGY BP Stent was intentionally designed  
with a fast-absorbing polymer to enable short DAPT

BIOABSORBABLE  
POLYMER



# HEAL

WITH CONFIDENCE



SYNERGY

This is a Dynamic Brochure  
Scan QR Code with your  
Smart Phone camera to learn more

# STUDYING DAPT



## Leading in Short DAPT

Supporting well-constructed prospective Short DAPT clinical trials with over **5,000 patients** to study the SYNERGY™ BP Stent in different complex patient populations.<sup>†</sup>

**SYNERGY BP Stent was Intentionally Designed to Enable Short DAPT and to Benefit High-Bleeding Risk Patients<sup>†</sup>**

### SENIOR\*

1-month DAPT in stable elderly patients  
6-month DAPT in ACS elderly patients

**1,200 PATIENTS**

SYNERGY BP Stent vs REBEL™ BMS

**Region(s):** Europe  
**Primary Endpoint:** TCT 2017



2-Year Data  
Now Available

### EVOLVE Short DAPT

3-month DAPT in HBR patients IDE Trial

**2,009 PATIENTS**

IDE Trial | SYNERGY BP Stent

**Region(s):** US, Europe,  
Japan, Brazil



0-3 Month Baseline Data  
Now Available

### IDEAL Left Main\*

4-month DAPT in SYNERGY BP Stent LM cohort  
12-month DAPT in Xience™ PP Stent LM cohort

**818 PATIENTS**

SYNERGY BP Stent vs Xience PP Stent

**Region(s):** Europe, UK



Completed Enrollment

### POEM\*

1-month DAPT in HBR patients

**1,023 PATIENTS**

SYNERGY BP Stent

**Region(s):** Italy



Ongoing Enrollment

### SYNIVUS-DAPT\*

1-month DAPT in HBR patients

**100 PATIENTS**

SYNERGY BP Stent  
IVUS

**Region(s):** US



Ongoing Enrollment

**Reduced DAPT could minimize medication costs, complications and improve patient satisfaction**

\* Investigator-Sponsored Study. Boston Scientific is not responsible for the collection, analysis, or reporting of the investigator-sponsored research output which is the sole responsibility of the investigators. Boston Scientific's involvement in investigator-sponsored research is limited to providing financial support for research that advances medical and scientific knowledge about our products.

<sup>†</sup> Please review the SYNERGY DFI for full instructions on DAPT.



<sup>†</sup> Please review the SYNERGY DFI for full instructions on DAPT.

## SENIOR TRIAL

### 1-Month and 6-Month DAPT in Elderly Patients

#### Safety Data at 2 Years

The SYNERGY™ BP Stent continued to show superior results versus REBEL™ BMS with short BMS-like DAPT regimen at 2 Years.

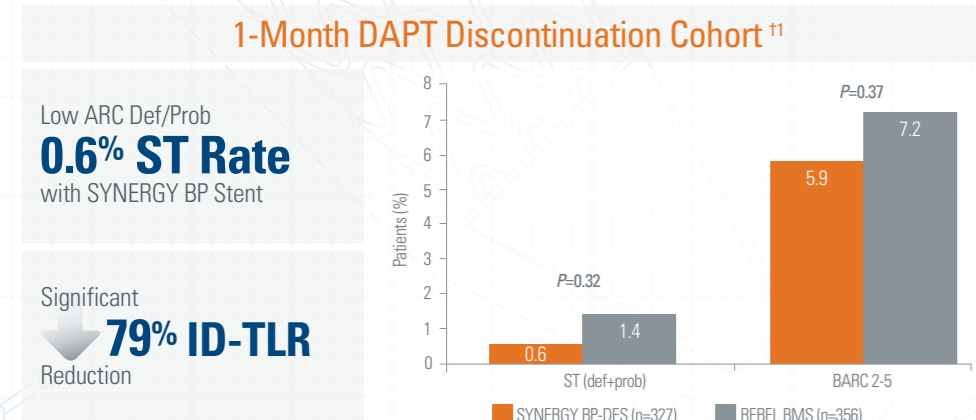
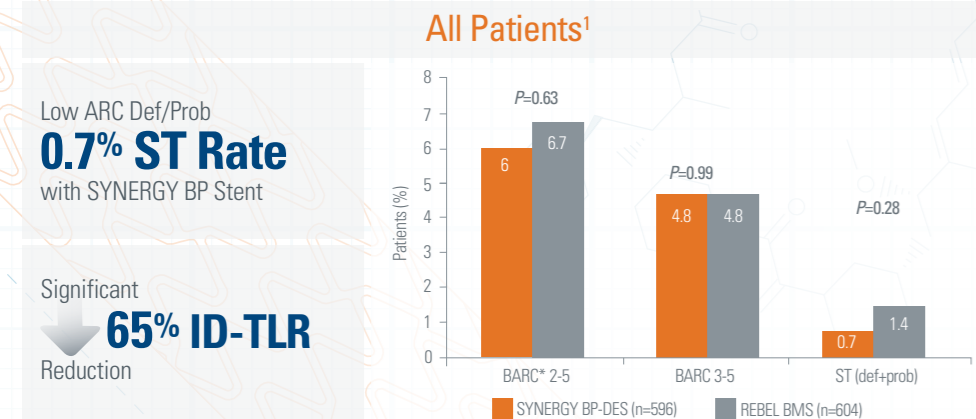


SENIOR Trial is a randomized, single-blind trial evaluating the SYNERGY BP Stent and the REBEL BMS in patients 75 years or older with a short duration of DAPT. Over 50% of patients enrolled received a 1-month DAPT regimen.

\* Bleeding Academic Research Consortium (BARC).  
† In patients eligible for 1-month DAPT in this study. Please review the SYNERGY DFI for full instructions on DAPT.  
† SENIOR Trial Presented by Olivier Varenne, MD, at TCT 2018.

#### Safety and Primary Endpoint Data at 1 Year

The SYNERGY BP Stent showed significantly lower MACCE<sup>‡</sup> rates versus REBEL BMS at 1 year.

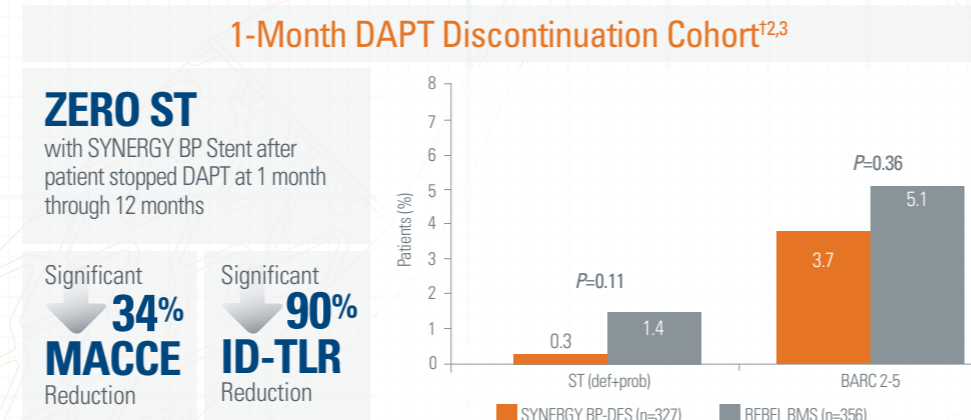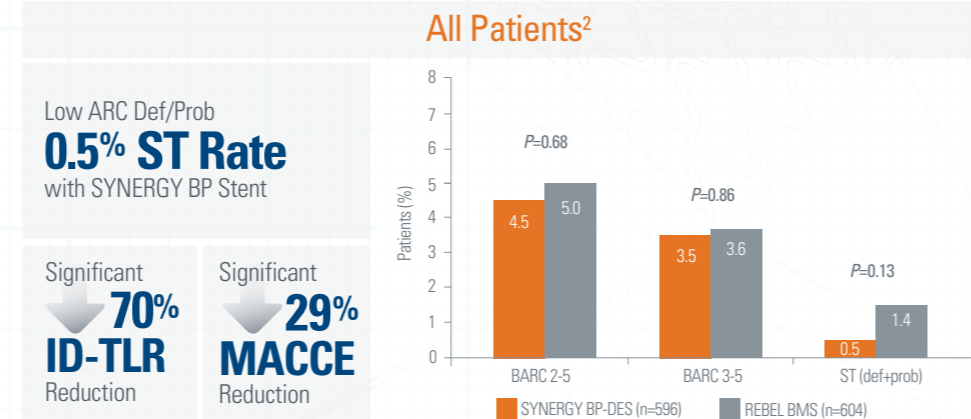

<sup>‡</sup> All-cause mortality, MI, stroke, and ischemia-driven TLR.  
<sup>2</sup> Varenne O, et al. Drug-eluting stents in elderly patients with coronary artery disease (SENIOR): a randomized single-blind trial. Lancet. 2018;391(10115):45-50. doi:10.1016/S0140-6736(17)32713-7.  
<sup>3</sup> SENIOR Trial Presented by Olivier Varenne, MD, at EuroPCR 2018.




## EVOLVE Short DAPT Trial

### 3-Month DAPT in High Bleeding Risk Patients

#### Clinical Outcomes at 3 Months<sup>4</sup>

The SYNERGY BP Stent showed extremely favorable outcomes in this complex patient group with significant bleeding risk:

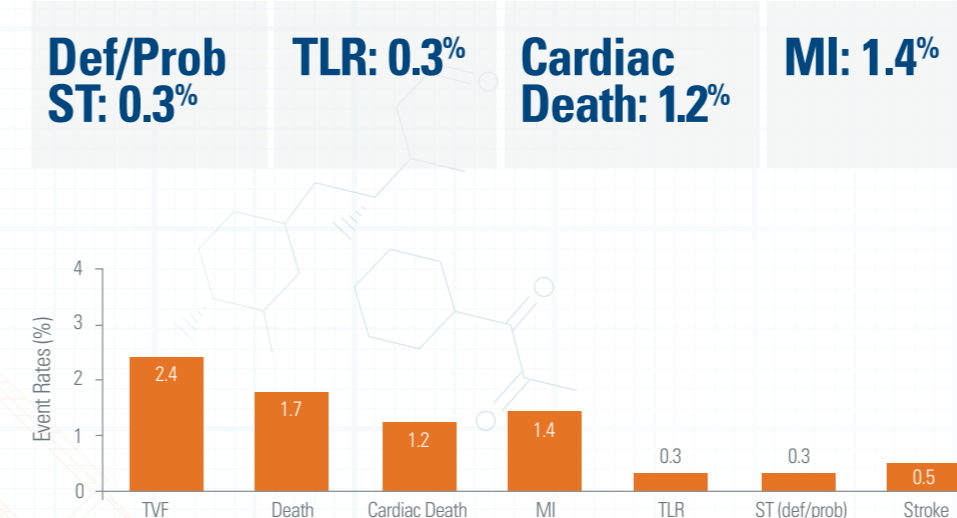

The 3-month DAPT data is very encouraging and we look forward to the 15-month primary endpoint results to be reported in late 2019.

EVOLVE Short DAPT Trial is a multicenter, single-arm trial evaluating safety of 3-month DAPT regimen in High Bleeding Risk (HBR) patients in 2009 patients at over 110 global sites. 67% patients are elderly patients with age ≥75 years.

<sup>4</sup> Presented by Ajay Kirtane, MD at TCT 2018.

## Continued DAPT Research

### IDEAL Left Main Trial

<b>Design</b>	Randomized trial in real world all-comers population accepted for Left Main PCI with 4-month DAPT with SYNERGY BP Stent versus 12-month DAPT with XIENCE PP Stent.
<b>Primary Endpoint</b>	Rate of MACE defined as composite of death from any cause, MI, stroke and ischemia-driven Target Vessel Revascularization (TVR) at 2 years. Primary endpoint results to be reported in mid-2019.

### POEM

<b>Design</b>	1-month DAPT in High Bleeding Risk (HBR) patients undergoing PCI with the SYNERGY BP Stent.
<b>Primary Endpoint</b>	Rate of MACE defined as composite of cardiac death, myocardial infarction, or definite/probable stent thrombosis at 1 year.

### SYNIVUS-DAPT

<b>Design</b>	1-month DAPT in HBR patients undergoing PCI with the SYNERGY BP Stent with intravascular ultrasound (IVUS).
<b>Primary Endpoint</b>	Rate of Cardiac Death and MI at 1 to 13 months.

"If you believe that short DAPT is preferable, we now have very strong evidence to select the SYNERGY Stent."

— Prof. Stefan James



# SYNERGY™

Everolimus-Eluting Platinum Chromium  
Coronary Stent System

# HEAL

WITH CONFIDENCE

All trademarks are the property of their respective owners. Prior to use, please review full device DFU for Indications, Contraindications, Warnings, Precautions, Adverse Events, and Operator's Instructions.

CAUTION: The law restricts these devices to sale by or on the order of a physician. Indications, contraindications, warnings and instructions for use can be found in the product labeling supplied with each device. Information for use only in countries with applicable health authority registrations. Material not intended for use in France.  
IC-598002-AB-MAY2019 - CreativeServices

**Boston  
Scientific**

Advancing science for life™

[www.bostonscientific-international.com](http://www.bostonscientific-international.com)

© 2019 Boston Scientific Corporation  
or its affiliates. All rights reserved.  
DINCAR2751EA