


AGENT™ DCB Paclitaxel-Coated PTCA Balloon Catheter
With **EMERGE™** Balloon Technology

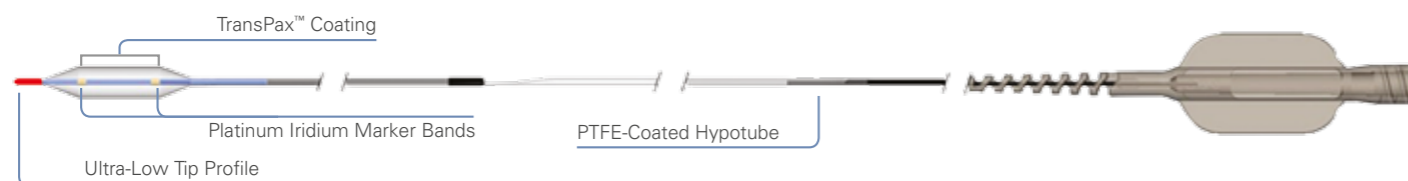

Ordering Information

Ref/Catalog Number	Order Number (GTIN)	Length	Diameter
H749 3922220121 0	08714729831402	12 mm	2.00 mm
H749 3922220151 0	08714729831419	15 mm	2.00 mm
H749 3922220201 0	08714729831426	20 mm	2.00 mm
H749 3922220301 0	08714729831433	30 mm	2.00 mm
H749 3922222121 0	08714729831457	12 mm	2.25 mm
H749 3922222151 0	08714729831464	15 mm	2.25 mm
H749 3922222201 0	08714729831471	20 mm	2.25 mm
H749 3922222301 0	08714729831488	30 mm	2.25 mm
H749 3922225121 0	08714729831501	12 mm	2.50 mm
H749 3922225151 0	08714729831518	15 mm	2.50 mm
H749 3922225201 0	08714729831525	20 mm	2.50 mm
H749 3922225301 0	08714729831532	30 mm	2.50 mm
H749 3922227121 0	08714729831556	12 mm	2.75 mm
H749 3922227151 0	08714729831563	15 mm	2.75 mm
H749 3922227201 0	08714729831570	20 mm	2.75 mm
H749 3922227301 0	08714729831587	30 mm	2.75 mm
H749 3922230121 0	08714729831600	12 mm	3.00 mm
H749 3922230151 0	08714729831617	15 mm	3.00 mm
H749 3922230201 0	08714729831624	20 mm	3.00 mm
H749 3922230301 0	08714729831631	30 mm	3.00 mm
H749 3922235121 0	08714729831709	12 mm	3.50 mm
H749 3922235151 0	08714729831716	15 mm	3.50 mm
H749 3922235201 0	08714729831723	20 mm	3.50 mm
H749 3922235301 0	08714729831730	30 mm	3.50 mm
H749 3922240121 0	08714729831808	12 mm	4.00 mm
H749 3922240151 0	08714729831815	15 mm	4.00 mm
H749 3922240201 0	08714729831822	20 mm	4.00 mm
H749 3922240301 0	08714729831839	30 mm	4.00 mm

AGENT™
Paclitaxel-Coated PTCA Balloon Catheter

**DRUG TRANSFER
REDEFINED**



**Outstanding Deliverability† with
the EMERGE™ Balloon Technology**


*Drug coating designed to deliver therapeutic drug dose in association with balloon angioplasty treatment.
† Bench testing as compared to Apex™ and Maverick™ balloons. Data on file at Boston Scientific.

Outstanding results in the first head-to-head comparison of drug coated balloons with different drug formulations


AGENT™ In-stent Restenosis Clinical Study Overview:

Patients (125) were randomized 1:1 to AGENT Paclitaxel-coated PTCA Balloon Catheter or SeQuent™ Please Paclitaxel-Releasing Coronary Balloon Catheter for the treatment of patients with in-stent restenosis of a previously-treated lesion of up to 28 mm in length (by visual estimate) in a native coronary artery 2.0 mm to 3.5 mm in diameter.

Primary Endpoint of Late Lumen Loss (LLL) Met¹

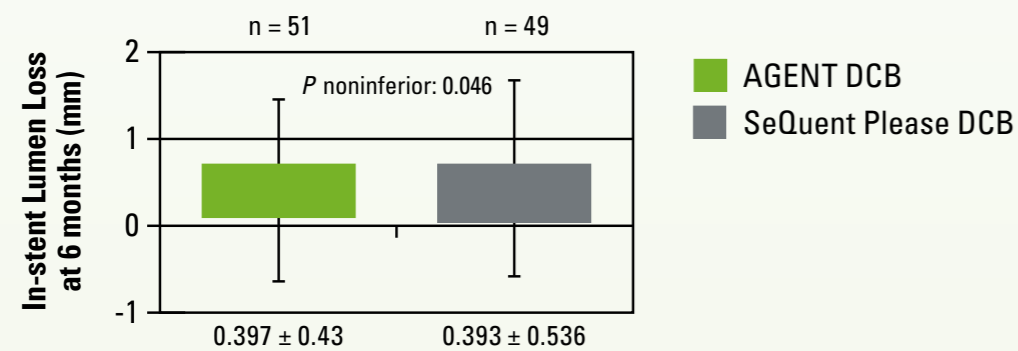

Numerically Lower Event Rates¹

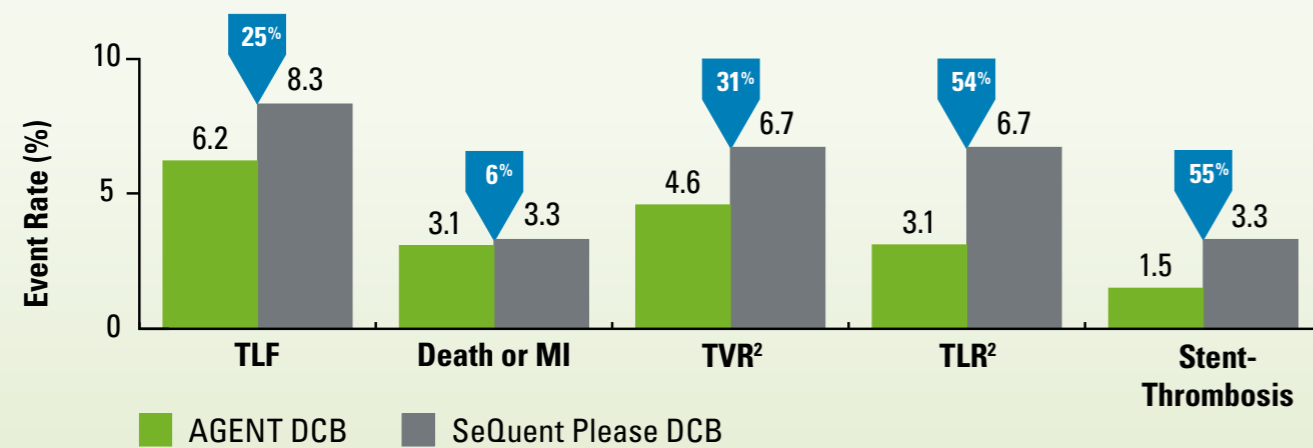

Binary event rate. All deaths were considered cardiac death. All *p*-values > 0.05.

1) Christian H. Drug-coated Balloons for the Treatment of Coronary In-stent Restenosis: A Randomised, Multicentre, Controlled Clinical Study; May 2017; Paris, France.
2) Data on file at Boston Scientific.

Optimized Drug Transfer

- TransPax™ coating ensures targeted delivery of Paclitaxel³
- Optimal dose of 2 µg/mm² compared to 3 µg/mm² of market leading DCBs⁴

Outstanding Deliverability⁵


AGENT™ DCB offers exceptional deliverability leveraging the EMERGE™ PTCA Catheter:

- Designed to navigate and cross challenging lesions
 - Ultra-low tip profile
 - Bi-segment inner shaft: flexible distal segment and pushable proximal segment

Enhanced Coating Integrity

- Balanced hydrophobic and hydrophilic properties of TransPax™ coating ensures balloon reaches the lesion with the optimal amount of drug for your patient
- Fewer particulates are lost distally during the procedure⁶

AGENT DCB generates less downstream materials when compared to competitors⁶

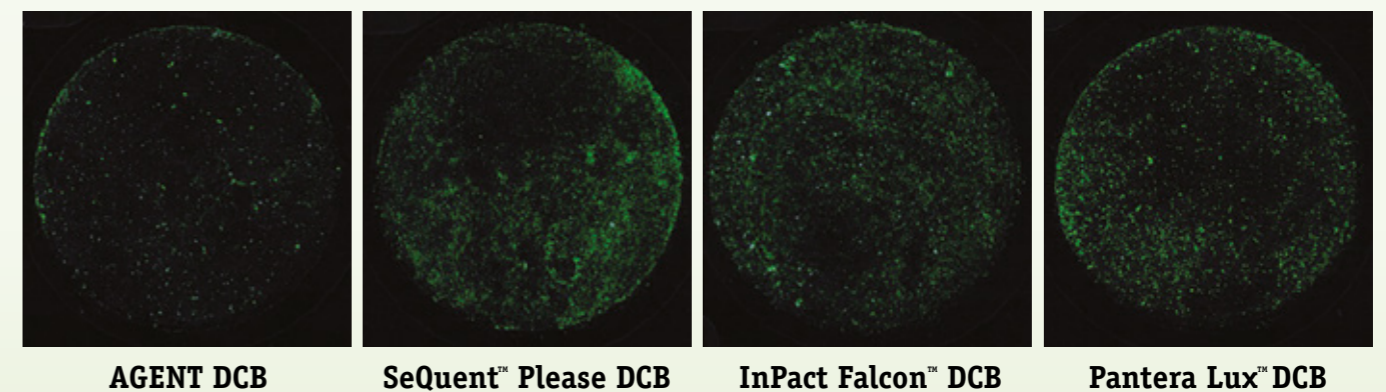

All particulate from insertion, delivery, inflation/deflation, and withdrawal captured on 5 µm filter.

3) Data on file at Boston Scientific. Pre-clinical results may not be necessarily indicative of clinical outcomes. Hemoteq Coating Process Validation by HPLC. Data on file at Hemoteq.
4) 3 µg/mm² dose for both B Braun SeQuent Please and Biotronik Pantera Lux per manufacturer's website.
5) Bench testing as compared to Apex™ and Maverick™ balloons. Data on file at Boston Scientific.
6) Method: balloons delivered in a coronary track model with fluid recirculation of 150 ml/min at T = 37 °C. Particulates are collected with a polycarbonate filter 5.0 µm x 47 mm (Sterilitech). Bench test results may not necessarily be indicative of clinical performance.