


Agent™

Paclitaxel-Coated PTCA Balloon Catheter

DRUG TRANSFER REDEFINED

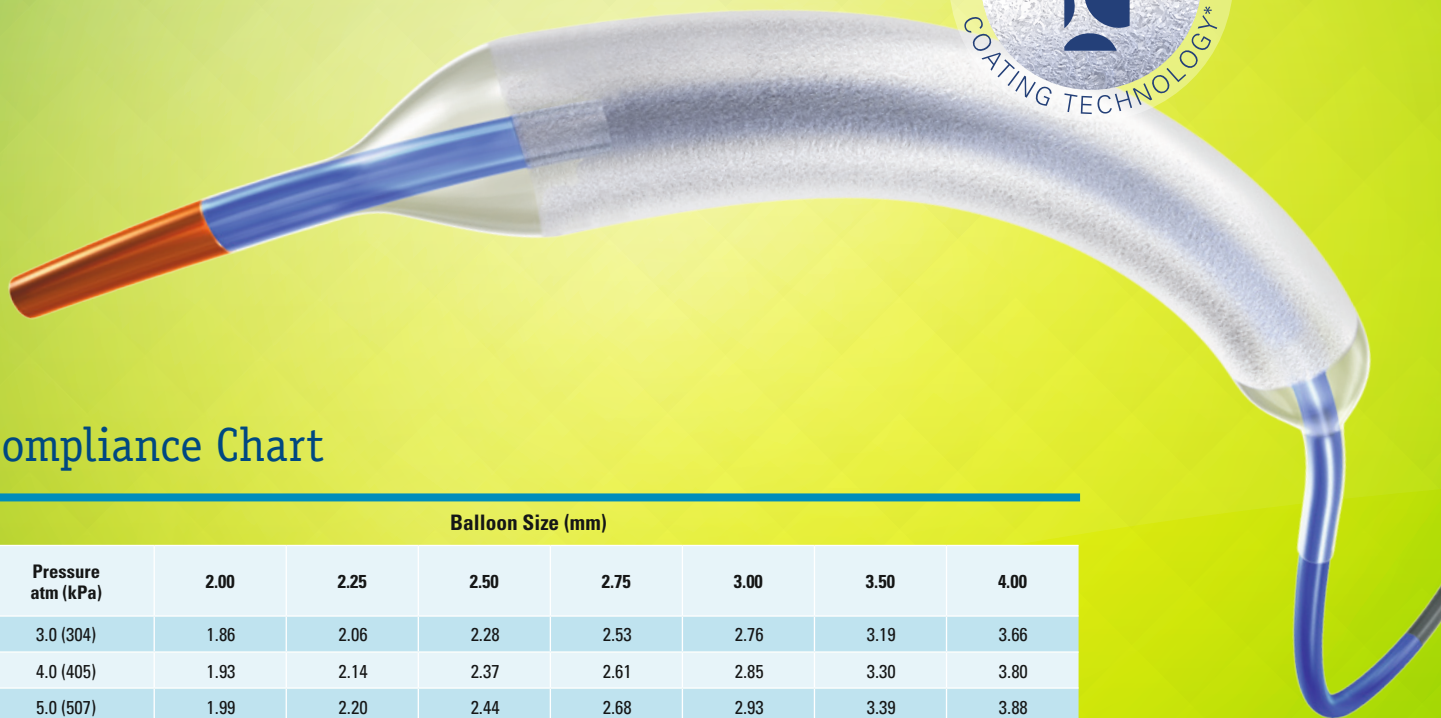

Compliance Chart

	Balloon Size (mm)						
Pressure atm (kPa)	2.00	2.25	2.50	2.75	3.00	3.50	4.00
3.0 (304)	1.86	2.06	2.28	2.53	2.76	3.19	3.66
4.0 (405)	1.93	2.14	2.37	2.61	2.85	3.30	3.80
5.0 (507)	1.99	2.20	2.44	2.68	2.93	3.39	3.88
6.0 (608)	2.03	2.26	2.50	2.75	3.00	3.46	3.96
7.0 (709)	2.07	2.31	2.55	2.81	3.06	3.52	4.04
8.0 (811)	2.10	2.34	2.59	2.85	3.11	3.57	4.09
9.0 (912)	2.13	2.38	2.62	2.88	3.15	3.61	4.14
10.0 (1013)	2.15	2.40	2.65	2.91	3.18	3.64	4.18
11.0 (1115)	2.18	2.42	2.67	2.94	3.21	3.68	4.22
12.0 (1216)	2.19	2.44	2.69	2.96	3.23	3.72	4.25
13.0 (1317)	2.21	2.46	2.72	2.99	3.26	–	–
14.0 (1419)	2.23	2.48	2.74	3.02	3.28	–	–




Nominal Pressure



Rated Burst Pressure. Do Not Exceed.

* Drug coating designed to deliver therapeutic drug dose in association with balloon angioplasty treatment.
Data on file at Boston Scientific.

Agent™ Paclitaxel-Coated PTCA Balloon Catheter

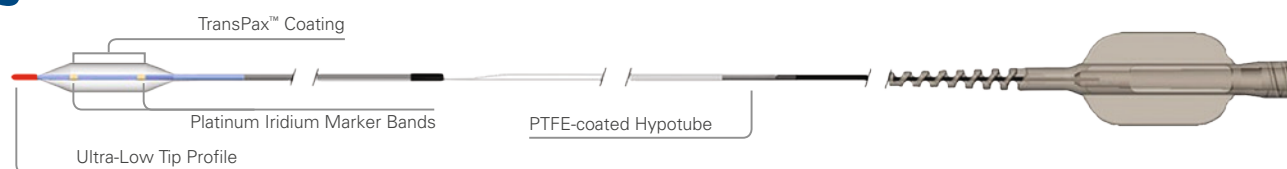

General Specifications and Materials List

Indications for Use	The Agent balloon catheter is indicated for Percutaneous Transluminal Coronary Angioplasty (PTCA) in the coronary arteries to treat in-stent restenosis (ISR) and de novo / small vessel disease.
Drug Coating	The TransPax drug coating is a proprietary formulation of Paclitaxel and a citrate ester excipient (acetyl tributyl citrate - ATBC). The Agent balloon catheter is designed to prevent hyperplasia of smooth muscle cells at the treated lesion site.
Drug Dose	2.0 µg per mm ² of the balloon surface
Recommended Inflation Time	At least 30 seconds
Antiplatelet Regimen	Recommended for 3 months after treatment
Available Balloon Lengths	In mm: 12, 15, 20, 30
Available Balloon Diameters	In mm: 2.00, 2.25, 2.50, 2.75, 3.00, 3.50, 4.00
Lesion Entry Profile	0.43 mm or 0.017"
Delivery System Effective Length	144 cm
Delivery System Port	Designed for 0.36 mm or 0.014" guidewire
Balloon Material	OptiLEAP™
Shelf Life	24 months
Sterilization	Ethylene oxide (EO)
Single/Multiple Use	Single Use
Guide Catheter Inner Diameter	1.42 mm or 0.056"
Guide Catheter Compatibility	5 F or 1.67 mm
Catheter Shaft Outer Diameter	1.67 mm or 0.0656"
Marker Band Material	Platinum-Iridium
Marker Band Placement	The outside edges of the marker bands indicate the balloon's shoulders and coated region

Product Ordering Information

Ø (mm)	Balloon Length (mm)			
	12	15	20	30
2.00	H74939222201210	H74939222201510	H74939222202010	H74939222203010
2.25	H74939222221210	H74939222221510	H74939222222010	H74939222223010
2.50	H74939222251210	H74939222251510	H74939222252010	H74939222253010
2.75	H74939222271210	H74939222271510	H74939222272010	H74939222273010
3.00	H74939222301210	H74939222301510	H74939222302010	H74939222303010
3.50	H74939222351210	H74939222351510	H74939222352010	H74939222353010
4.00	H74939222401210	H74939222401510	H74939222402010	H74939222403010

Boston Scientific
Advancing science for life™

All trademarks are the property of their respective owners.

CAUTION: The law restricts these devices to sale by or on the order of a physician. Indications, contraindications, warnings and instructions for use can be found in the product labelling supplied with each device. Information for the use only in countries with applicable health authority product registrations. Information contained herein is for distribution outside the United States, France, and Japan. Illustrations for information purposes – not indicative of actual size or clinical outcome.

Agent Paclitaxel-Coated PTCA Balloon Catheter is manufactured by Hemotek AG and distributed by Boston Scientific Corporation.

bostonscientific-international.com

Copyright © 2015 by
Boston Scientific Corporation
or its affiliates. All rights reserved.

IC-236507-AB OCT2015