



SpyGlass™ DS Direct Visualization System

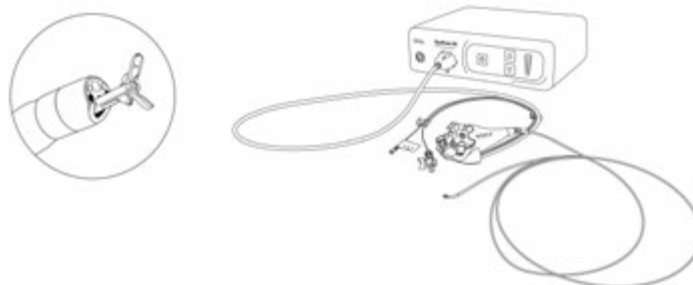
➤ Disposable Devices	39
➤ Capital Equipment	39

SpyGlass Direct Visualization System




➤ Disposable and Reusable Devices	40
➤ Capital Equipment	40

SpyGlass™ DS Direct Visualization System

Capital Equipment & Devices



Disposable Devices

Order Number	GTIN	Description	Packaging
M00546600	08714729863236	 SpyScope™ DS Access & Delivery Catheter	Each
M00546270	08714729764458	 SpyBite™ Biopsy Forceps	Each
M00546451	10677964060905	 SpyGlass Irrigation Tube Set	Box 10

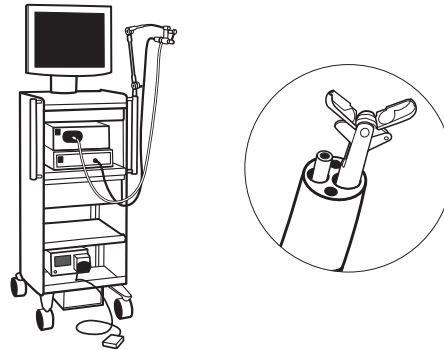
Capital Equipment

Order Number	GTIN	Description	Packaging
M00546650	08714729874348	SpyGlass DS Digital Controller	Please contact your Boston Scientific Sales Representative for ordering information.




For more information on ordering a compatible EHL or Laser Probe for the SpyGlass DS Direct Visualization System, please contact your Boston Scientific Representative.

SpyGlass™ Direct Visualization System

Capital Equipment & Devices



Disposable and Reusable Devices¹

Order Number	GTIN	Description	Packaging
M00546030	08714729764441	SpyGlass Direct Visualization Probe	Each
M00546230	08714729764434	 SpyScope™ Access & Delivery Catheter	Each
M00546270	08714729764458	 SpyBite™ Biopsy Forceps	Each
M00546451	10677964060905	 SpyGlass Irrigation Tube Set	Box 10

Capital Equipment

Order Number	GTIN	Description	Packaging
M00546100	10845854043158	SpyGlass Camera	Each
M00546190	10845854043202	SpyGlass Lightsource	Each
M00546210	10845854043264	SpyGlass Light Cable	Each
M00546040	08714729773566	SpyGlass Ocular	Each
M00546140	08714729773573	Irrigation Pump with Foot Switch	Each
M00546060	08714729779629	SpyGlass Storage Tray – Large ²	Each
M00546050	08714729780250	SpyGlass Storage Tray – Small ²	Each

¹ The SpyScope Access and Delivery Catheter, SpyBite Forceps and Irrigation Tubing are single-use devices. The SpyGlass Direct Visualization Probe is a reusable device that has been validated up to 20 reprocessing cycles of high level disinfection. The true number of procedural uses, however, will depend on how the SpyGlass Probe is handled. Fiberoptics are very sensitive and need delicate handling.

² Purchase of a minimum of two storage trays is recommended. Large storage trays (M00546060) are recommended unless account reprocesses in an Olympus™ Medivators™ Machine, into which the large storage trays will not fit. In this case, small storage trays should be ordered (M00546050).

Notes and Future Product Updates

Notes and Future Product Updates

