

# TRUEtome™

Cannulating Sphincterotome

About

Device Features

Therapeutic Accessories

Ordering

## Delivering Performance and Choice

Optimizing wire-guided cannulation and  
the treatment of pancreatobiliary diseases


Boston  
Scientific



## ▶ About TRUEtome

TRUEtome is the Cannulating Sphincterotome that has the potential to bring utility to every endoscopic retrograde cholangiopancreatography (ERCP).

Designed for performance, the TRUEtome Sphincterotome is for the physician who prefers long wire devices and values having options when it comes to guidewire selection.

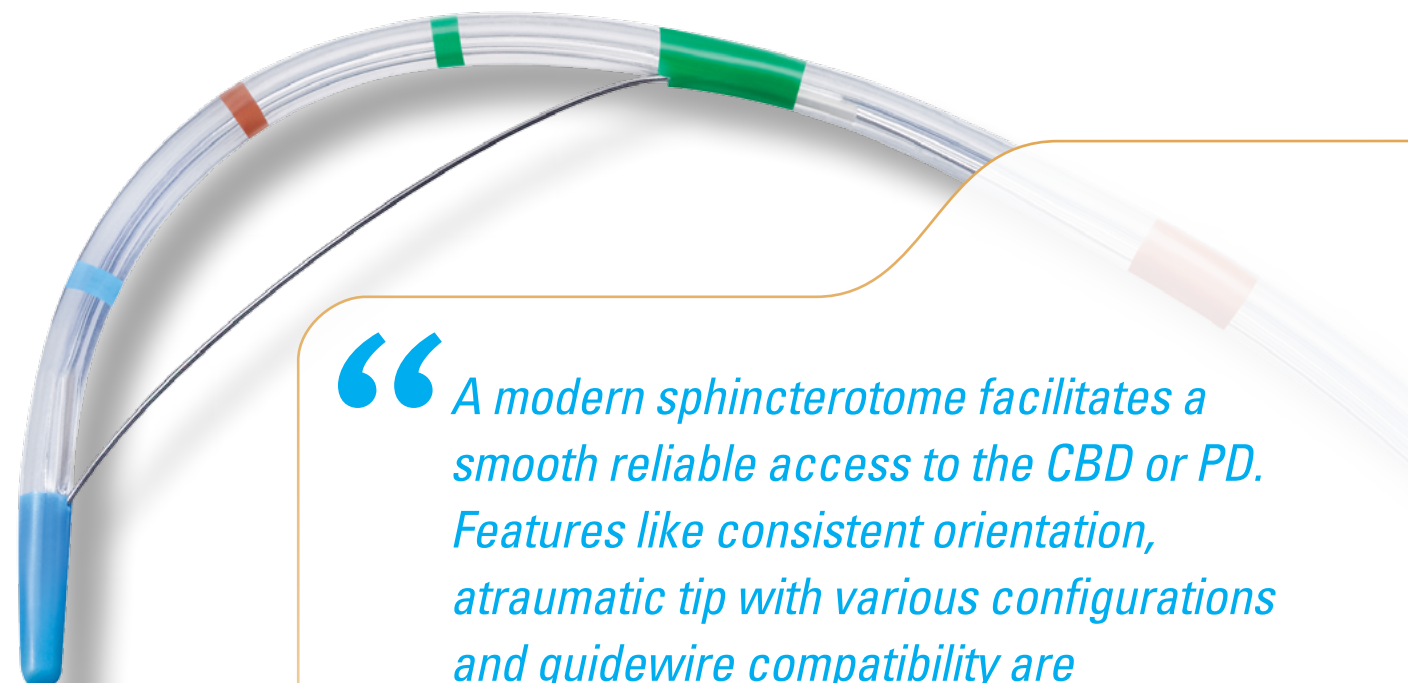

“A modern sphincterotome facilitates a smooth reliable access to the CBD or PD. Features like consistent orientation, atraumatic tip with various configurations and guidewire compatibility are essential for successful cannulation. The TRUEtome™ steerable tip can be helpful for aligning the cut wire before sphincterotomy and can simplify a targeted positioning of a guidewire to the desired duct.”

**Prof. Horst Neuhaus**  
EVK, Düsseldorf, Germany

## ▶ Device Features

1 of 3



**Center Guidewire Lumen** design allows the guidewire to extend from the center of the sphincterotome to aid in positioning and facilitates wire-guided cannulation.\*

**Wire-guided Cannulation is known to reduce the risk of post-ERCP pancreatitis compared with the standard contrast injection method.<sup>1</sup>**



**Center Injection Lumen** design allows injection of contrast to exit from the center of the catheter enabling delivery of contrast to the intended duct.

\*Does not apply to 4.9F (1.63mm) diameter.

1. Cennamo et al. Can a Wire-Guided Cannulation Technique Increase Bile Duct Cannulation Rate and Prevent Post-ERCP Pancreatitis?: A Meta-Analysis of Randomized Controlled Trials. The American Journal of Gastroenterology, 2009.



## ▶ Device Features

◀ 2 of 3 ▶

Sphincterotome design accommodates **Multiple Guidewire Diameters** from 0.018-0.035in and allows for use of multiple guidewires during a procedure.\*

### Sphincterotome Multiple Tip Sizes

accommodate varying patient anatomies and facilitates cannulation:



**3.9F**

(0.018-0.025in)



**4.4F**

(0.018-0.035in)



**4.9F**

(0.018-0.035in)



\*TRUEtome 3.9F Sphincterotome accepts a maximum guidewire of 0.025in

3.9F = 1.30mm

4.4F = 1.47mm

4.9F = 1.63mm

0.018in = 0.46mm


0.025in = 0.64mm

0.035in = 0.89mm

## ▶ Device Features

◀ 3 of 3

**Controlled Steerability** provides optimal positioning for ERCP cannulation and sphincterotomy. Steerability enables intraductal selective cannulation to aid in accessing the pancreatobiliary tree.

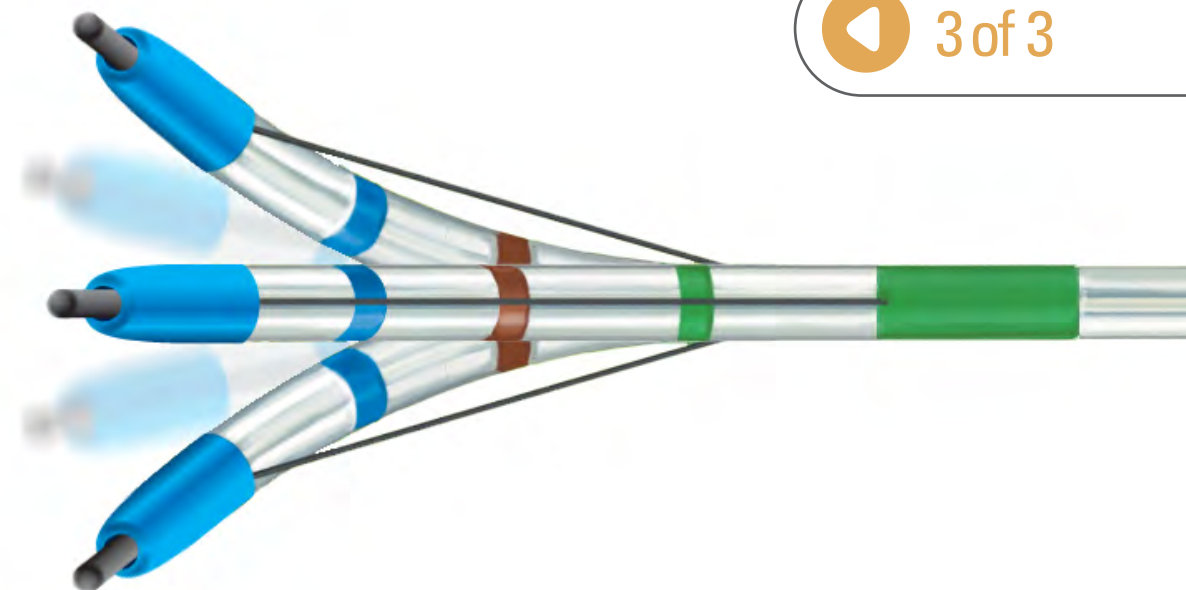

**Handle Brake** helps maintain catheter bow for all tip sizes and added control during sphincterotomy.





## ▶ Therapeutic Accessories

1 of 2 ▶

### Boston Scientific is committed to improving patient care

for the management of pancreatobiliary diseases, including: gall bladder and biliary stones; pancreatic stones; cholangiocarcinoma; pancreatic cancer; primary sclerosing cholangitis; and sphincter of oddi dysfunction.

“The sphincterotome is one of the most important tools in ERCP. A good sphincterotome has to be designed for easy cannulation, safe sphincterotomy and for optimal device exchange. It has to be compatible with different endoscopes and adaptable to altered patient anatomies in order to match the constantly evolving ERCP techniques.”

**Prof. Guido Costamagna** Policlinico Universitario, A. Gemelli, Rome, Italy


### Through innovation and continuous improvement

Boston Scientific offers a wide range of therapeutic accessories for the diagnosis and treatment of pancreatobiliary stone and stricture management.


## ▶ Therapeutic Accessories

◀ 2 of 2


The TRUEtome Sphincterotome works effectively with these devices:




Trapezoid™ RX  
Retrieval Basket




Extractor™ Pro  
Retrieval Balloon




CRE™ Balloon for Dilation  
Assisted Stone Extraction




Combo Cath™  
Cytology Brush




Hurricane™ RX  
Dilation Balloon




Advanix™ Biliary Stent with  
NaviFlex™ RX Delivery System



WallFlex™ Biliary RX  
Metal Stents



Dreamwire™ Guidewire



Hydra Jagwire™ Guidewire

### Access Devices

▶ Visit: [www.bostonscientific.com/endo-resources](http://www.bostonscientific.com/endo-resources)



## Ordering Information

TRUEtome Cannulating Sphincterotomes are available in three tapered tip sizes to accommodate varying patient anatomies.

Order Number (Box 1)	Order Number (Box 10)	Order Number (Box 20)	Product Description	Cut Wire Length (mm)	Tip Length (mm)	Distal Tip O.D. (F)	Recommended Guidewire Diameter (in)
M00584150	M00584151	M00584152	TRUEtome 49 Sphincterotome	20	5	4.9	0.018-0.035
M00584160	M00584161	M00584162	TRUEtome 49 Sphincterotome	30	5	4.9	0.018-0.035
M00584170	M00584171	M00584172	TRUEtome 44 Sphincterotome	20	5	4.4	0.018-0.035
M00584180	M00584181	M00584182	TRUEtome 44 Sphincterotome	30	5	4.4	0.018-0.035
M00584190	M00584191	M00584192	TRUEtome 39 Sphincterotome	20	5	3.9	0.018-0.025
M00584120	M00584121	M00584122	TRUEtome 39 Sphincterotome	30	5	3.9	0.018-0.025

3.9F = 1.30mm      0.018in = 0.46mm  
 4.4F = 1.47mm      0.025in = 0.64mm  
 4.9F = 1.63mm      0.035in = 0.89mm

**Boston  
Scientific**

Advanix, Combo Cath, CRE, Dreamwire, Extractor, Hurricane, Hydra Jagwire, NaviFlex, Trapezoid, TRUEtome, WallFlex are unregistered or registered trademarks of Boston Scientific Corporation or its affiliates.

All cited trademarks are the property of their respective owners. CAUTION: The law restricts these devices to sale by or on the order of a physician. Indications, contraindications, warnings and instructions for use can be found in the product labelling supplied with each device. Information for the use only in countries with applicable health authority product registrations. Produced by Gosling.

© 2013 Boston Scientific Corporation or its affiliates. All rights reserved.  
 ENDO-114206-AA / ENDO-129402-AA  
 Dec 2012