



Hot AXIOS™

Stent and Electrocautery Enhanced Delivery System

**Boston
Scientific**
Advancing science for life™

Advancing Pancreaticobiliary Disease Management

Select a Menu Option Below

**FEATURES &
BENEFITS**

**EXPANDING
INNOVATION**

**ORDERING
INFORMATION
& RESOURCES**

Whether cases are simple or complex,
the standard of care should be anything but standard.



The Hot AXIOS Stent and Electrocautery Enhanced Delivery System provides a simpler and faster treatment option for patients, we can now provide an endoscopic solution that provides relief for these patients using one device in a single setting.

Kenneth Binmoeller, M.D.

California Pacific Medical Center, San Francisco, CA and the inventor of the AXIOS System.



**Because today's barriers are
tomorrow's breakthroughs.**



Features & Benefits


Enabling an Endoscopic Solution

The Hot AXIOS™ Stent and Electrocautery Enhanced Delivery System


was the first stent indicated for indicated to facilitate transgastric or transduodenal endoscopic drainage of:

- a pancreatic pseudocyst or a walled-off necrosis with $\geq 70\%$ fluid content
- gallbladder in patients with acute cholecystitis who are at high risk or unsuitable for surgery
- the bile duct after failed ERCP in patients with biliary obstruction due to a malignant stricture

The cautery-enhanced access and delivery catheter is advanced through the tissue creating a transluminal conduit between the stomach or duodenal wall and the pancreatic pseudocyst where the pre-loaded stent is deployed to provide drainage.

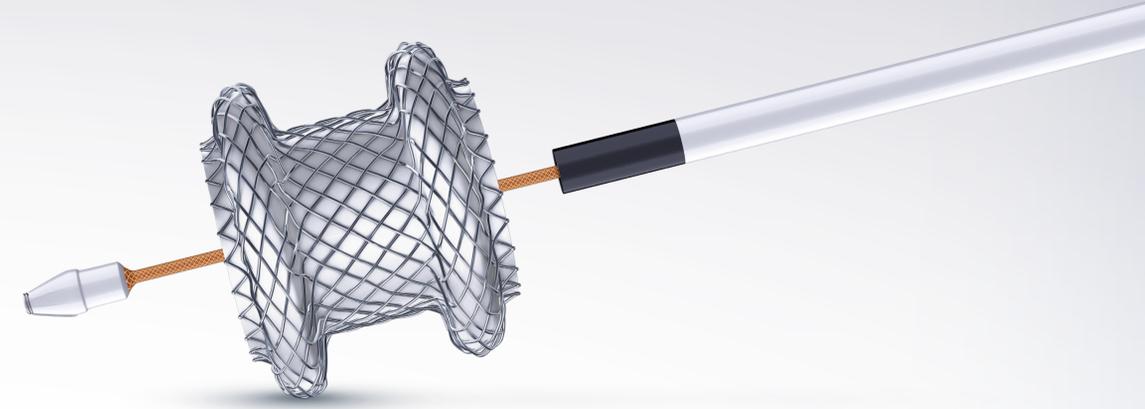


Stent Design

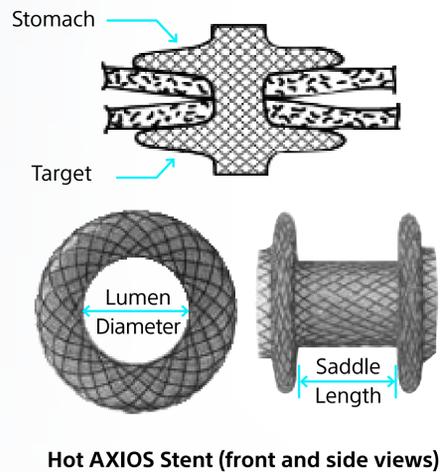

- Proprietary one-step combined diathermic ring and cut-wire provides access into target tissue
- MRI conditional, fully covered self-expanding metal stent pre-loaded in the delivery catheter
- Perpendicular flanges secure tissue layers and help prevent migration
- Six sizes available, with the largest featuring a 20 mm lumen for drainage
- The four largest diameter LAMS enable drainage and allow passage of an endoscope through the stent for additional therapeutic procedures including cystoscopy, irrigation and debridement.

Potential Clinical Benefits

Previous available technologies for endoscopic management of pancreatic pseudocysts were not originally designed or intended for this type of treatment.

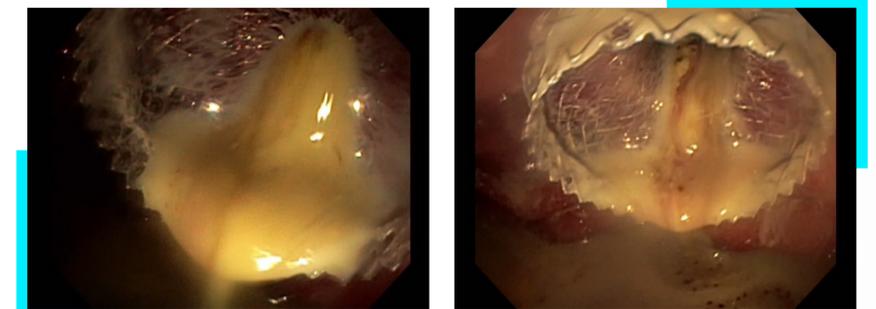

Images provided by Dr. Adler.

The 20 mm Hot AXIOS Stent size was ideal for my patient with a large PFC/WON as it allowed rapid drainage of solid and liquid contents and will greatly facilitate endoscopic necrosectomy going forward.

Douglas G Adler MD, FACP, AGAF, FASGE

University of Utah School of Medicine,
Huntsman Cancer Center, Salt Lake City, Utah, U.S.A.



Expanding Innovation in EUS

Click / Tap on a milestone below to learn more (Internet Required)




2011
Expect™ Endoscopic
Ultrasound (EUS)
Aspiration Needle




2011
AXIOS™
Stent & Delivery System*

- indicated for use to facilitate transgastric or transduodenal endoscopic drainage of a pancreatic pseudocyst or a walled-off necrosis with $\geq 70\%$ fluid content.



2013
Hot AXIOS™ Electrocautery Enhanced Stent & Delivery System


- Providing an endoscopic treatment option as a potential alternative to surgery for patients suffering from pancreatic pseudocysts and WON¹.
- The first metal stent indicated for use to facilitate transgastric or transduodenal endoscopic drainage of:
 - a pancreatic pseudocyst or a walled-off necrosis with $\geq 70\%$ fluid content
 - gallbladder in patients with acute cholecystitis who are at high risk or unsuitable for surgery
 - the bile duct after failed ERCP in patients with biliary obstruction due to a malignant stricture



[Learn More](#)

2016
Acquire™ FNB Device

- May reduce the need for repeat procedures
- Franseen needle tip is designed to capture larger biopsy samples²



[Learn More](#)

2024
Acquire™ S
Endoscopic Ultrasound Fine
Needle Biopsy (FNB) Device

designed for ease-of-puncture¹ and to help maximize diagnostic yield without compromising the quality of core tissue samples to obtain an accurate diagnosis.²



[Learn More](#)

2011

2012

2013

2014


2016

2017

2019

2024

2012
Expect™
19ga
Flex EUS
Aspiration
Needle

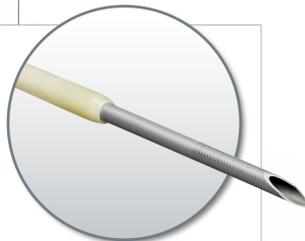

2014
Expect™ Slimline
(SL) Needle



2016
20mm Hot AXIOS™
Stent and
Electrocautery
Enhanced Delivery
System Featuring a
 larger lumen for drainage.



[Discover our Hot AXIOS' learning paths](#)

2017
Expect™ Slimline Needle
Expanded Indications,
 including the delivery of
 injectable materials (fluids)
 or fiducials into tissue or for
 passage of accessory devices.



[Learn More](#)

2019
15x15 mm
Hot AXIOS™
Stent and
Electrocautery
Enhanced
Delivery
System



Ordering Information & Resources

Hot AXIOS™ Stent System



The Hot AXIOS™ Stent and Electrocautery Enhanced Delivery System is available in the following stent configurations. Each Hot AXIOS™ Stent comes pre-loaded into the Hot AXIOS™ Delivery System.

Product Code	Description	Flange Diameter (mm)	Lumen Diameter (mm)	Saddle Length (mm)	Catheter OD (Fr)	Catheter Working Length (cm)	Catheter Total Length (cm)
M005 53520	1 Hot AXIOS System with 6 x 8 Stent	14	6	8	9	138	144
M005 53530	1 Hot AXIOS System with 8 x 8 Stent	17	8	8	9	138	144
M005 53540	1 Hot AXIOS System with 10 x 10 Stent	21	10	10	10.8	138	144
M005 53550	1 Hot AXIOS System with 15 x 10 Stent	24	15	10	10.8	138	144
M005 53570*	1 Hot AXIOS System with 15 x 15 Stent	24	15	15	10.8	138	144
M005 53560	1 Hot AXIOS System with 20 x 10 Stent	29	20	10	10.8	138	144

*The 15 x 15 Hot AXIOS Stent and Electrocautery-Enhanced Delivery System is indicated for use to facilitate transgastric or transduodenal endoscopic drainage of a pancreatic pseudocyst or a walled-off necrosis with ≥ 70% fluid content.

Additional Resources




Download the **Product Catalogue**

[PRODUCT CATALOGUE ▶](#)



Visit the HPB Portal for information about Boston Scientific's **HPB devices, services and solutions.**

[WWW.BOSTONSCIENTIFIC.EU ▶](http://WWW.BOSTONSCIENTIFIC.EU)



Visit **EDUCARE** to watch various educational EUS programs, case studies, and lectures

[EDUCARE ▶](#)



[FOLLOW US ON LINKEDIN ▶](#)



[FOLLOW US ON X ▶](#)





1. Data on File. Windchill document #92959483 Bench Test Data. Acquire S Puncture Force Claims Technical Report A. The testing was performed by BSC. Data on file. Test Method Summary: P<.001, 15 unit sample size for each needle type and performed three consecutive punctures with each needle in a synthetic gel block material to assess puncture force required after three punctures. The Acquire 22ga EUS FNB Needle was tested with the stylet retracted for puncture with the needle tip. The Acquire S 22ga EUS FNB Needle was tested using the stylet in the forward position for puncture with the stylet. Needles tested are the Acquire 22ga EUS FNB Needle (Boston Scientific Corporation, Marlborough, MA) and Acquire S 22ga EUS FNB Needle (Boston Scientific Corporation, Marlborough, MA). Bench testing results may not necessarily be indicative of clinical performance.
2. Kaneko J, Ishiwatari H, Sasaki K, et al. Macroscopic on-site evaluation of biopsy specimens for accurate pathological diagnosis during EUS-guided fine needle biopsy using 22-G Franseen needle. Endosc Ultrasound. 2020;9(6):385-391.

The Hot AXIOS 15x15 Stent and Delivery System is indicated for use to facilitate transgastric or transduodenal endoscopic drainage of a pancreatic pseudocyst or a walled-off necrosis with $\geq 70\%$ fluid content.

The Hot AXIOS Stent and Electrocautery-Enhanced Delivery System is indicated for use to facilitate transgastric or transduodenal endoscopic drainage of:

- gallbladder in patients with acute cholecystitis who are at high risk or unsuitable for surgery
- the bile duct after failed ERCP in patients with biliary obstruction due to a malignant stricture

All trademarks are the property of their respective owners.

Indications, Contraindications, Warnings and Instructions for Use can be found in the product labeling supplied with each device.

CAUTION: The law restricts these devices to sale by or on the order of a physician. Indications, contraindications, warnings and instructions for use can be found in the product labelling supplied with each device. Information for use only in countries with applicable health authority registrations. Material not intended for use in France. Product available in the European Economic Area (EEA) only. Please check availability with your local sales representative or customer service.

**Boston
Scientific**
Advancing science for life™

www.bostonscientific.eu

© 2024 Boston Scientific Corporation
or its affiliates. All rights reserved.

ENDO-622702-AC