




**Interlock™ -18 Fibered IDC™ Occlusion System**

<b>Standard Length 2D Configurations</b>						
<b>UPN</b>	<b>Description</b>	<b>Diameter (mm)</b>	<b>Length (cm)</b>	<b>Shape</b>		
M001361480	Interlock - 18 Coil	2	4	2D		
M001361490	Interlock - 18 Coil	2	6	2D		
M001361500	Interlock - 18 Coil	3	6	2D		
M001361510	Interlock - 18 Coil	3	12	2D		
M001361520	Interlock - 18 Coil	4	8	2D		
M001361530	Interlock - 18 Coil	4	15	2D		
M001361540	Interlock - 18 Coil	5	8	2D		
M001361550	Interlock - 18 Coil	5	15	2D		
M001361560	Interlock - 18 Coil	6	10	2D		
M001361570	Interlock - 18 Coil	6	20	2D		
M001361580	Interlock - 18 Coil	8	20	2D		
M001361590	Interlock - 18 Coil	10	20	2D		
M001361600	Interlock - 18 Coil	10	30	2D		
M001361610	Interlock - 18 Coil	12	20	2D		
M001361620	Interlock - 18 Coil	12	30	2D		
M001361630	Interlock - 18 Coil	14	20	2D		
M001361640	Interlock - 18 Coil	14	30	2D		
<b>Long Length 2D Configurations</b>						
<b>UPN</b>	<b>Description</b>	<b>Diameter (mm)</b>	<b>Length (cm)</b>	<b>Shape</b>		
M001361920	Interlock - 18 Coil	10	50	2D		
M001361930	Interlock - 18 Coil	14	50	2D		
M001361940	Interlock - 18 Coil	18	50	2D		
M001361950	Interlock - 18 Coil	20	50	2D		
M001361960	Interlock - 18 Coil	22	60	2D		
<b>Diamond Configurations</b>						
<b>UPN</b>	<b>Description</b>	<b>Diameter (mm)</b>	<b>Length (cm)</b>	<b>Shape</b>		
M001361740	Interlock - 18 Coil	2/3	2.3	Diamond		
M001361750	Interlock - 18 Coil	2/4	4.1	Diamond		
M001361760	Interlock - 18 Coil	2/5	5.8	Diamond		
M001361770	Interlock - 18 Coil	2/6	8	Diamond		

**Direxion Torqueable Microcatheter**

<b>UPN</b>	<b>Order Number</b>	<b>Usable Length (cm)</b>	<b>Tip Shape</b>	<b>RO Markers</b>
M001195320	19-532	130	Straight	2
M001195340	19-534	2	Bern	2

Illustrations are not necessary to scale. All images are property of Boston Scientific.

0.018-inch (0.457-mm)

Interlock and Fibered IDC are unregistered trademarks of Boston Scientific Corporation or its affiliates.

All cited trademarks are the property of their respective owners. CAUTION: The law restricts these devices to sale by or on the order of a physician. Indications, contraindications, warnings and instructions for use can be found in the product labelling supplied with each device. Information for the use only in countries with applicable health authority product registrations.

PI-213401-AA JAN 2014 Printed in Germany by medicalvision.

**Boston Scientific**  
Advancing science for life™


www.bostonscientific-international.com

© 2013 Boston Scientific Corporation or its affiliates. All rights reserved. DINONC3503EA

**Boston Scientific**  
Advancing science for life™

**Interlock™ -18 Coil**  
Fibered IDC™ Occlusion System

*A little smaller and  
A lot Bigger*

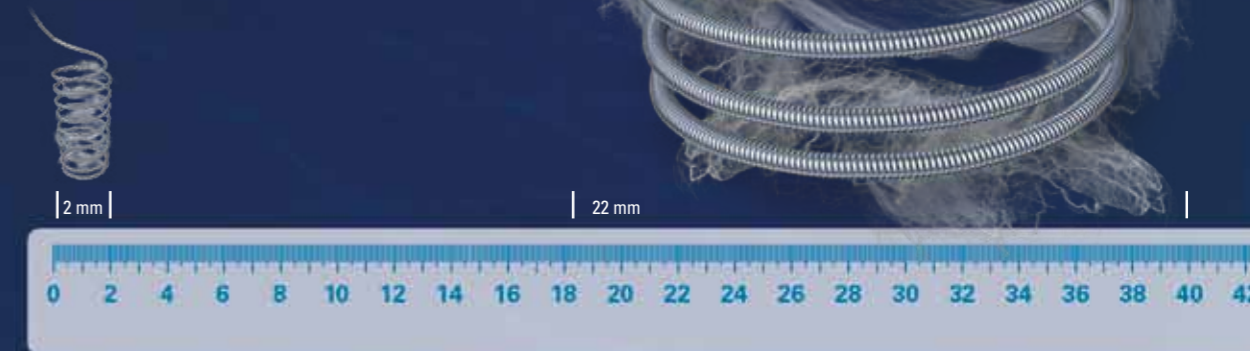


Images are not drawn to scale



# Lock In Accuracy, Power and Precision

In a prospective, randomized, single-center study, the use of the Interlock™ Fibered IDC™ Occlusion System for embolization of the GDA allowed investigators to place significantly fewer coils.

## Number of Coils Used Per Procedure

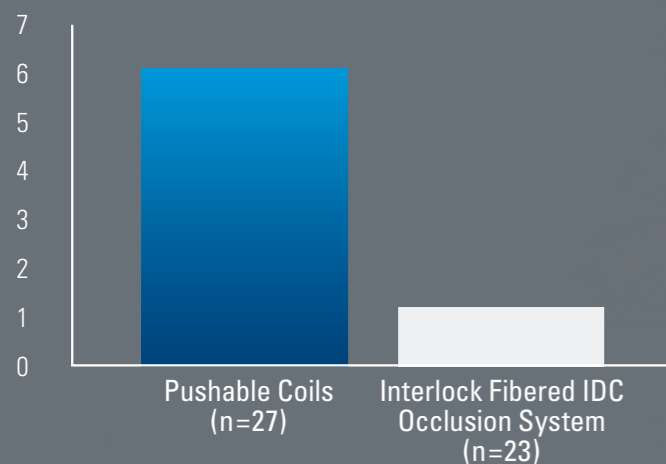

Dudek, et al, Embolization of the Gastroduodenal Artery Before Selective Internal Radiotherapy: A Prospectively Randomized Trial Comparing Standard Pushable Coils with Fibered Interlock Detachable Coils. CVIR, April 14, 2010.

- 83.6% of cases (19 of 23) achieved complete occlusion with one Interlock Fibered IDC Occlusion Coil.
- A shorter procedure time was observed for procedures utilizing detachable coils when compared to pushable coils.
- No coil migration was observed in the detachable coil group, whereas one incidence of migration was observed in the pushable coil group.

## Accuracy

Interlocking arms offer physicians the potential for greater control, precision and retractability.

## Precision\*


Broad range of product sizes including 2–22 mm diameters and up to 60 cm lengths.

## Power

Highly thrombogenic fibering configuration and long coil lengths engineered for fast and reliable vessel occlusion.

\* For placement accuracy and control in delivery you can now use Direxion™ torqueable microcatheter with Double Radiopaque Marker.

### Microcatheter with 1 Radiopaque marker

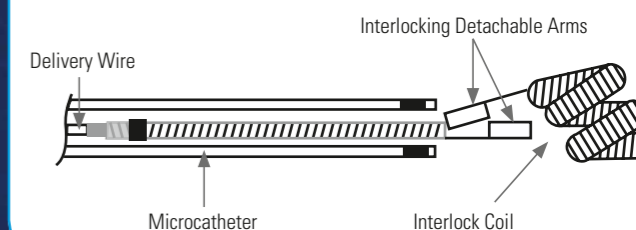

### Microcatheter Double Marker

