

2024

# Rhythm Management Product Performance Report

Q3 Edition



RESONATE™  
Family of ICDs AND CRT-Ds



ACCOLADE™  
Family of Pacemakers

INGEVITY™ +  
Pacing Lead



CRM Quality Pledge

I improve  
the quality  
of patient care  
and all things  
Boston Scientific

## Advancing Science for Life.

For over forty years, meaningful innovation at Boston Scientific Rhythm Management has helped patients live healthier, longer lives. We are committed to providing performance data which are accurate, transparent and responsive to topics of contemporary clinical interest. This Q3 2024 report includes data through July 2nd, 2024.

Boston Scientific provides performance data for pulse generators and leads that meets or exceeds the 2014 revision of ISO 5841-2: 2014 (E), the AdvaMed Industry Guidance for Uniform Reporting of Clinical Performance, and addresses recommendations from the Heart Rhythm Society Task Force.

This report provides the most comprehensive presentation of rhythm management product performance data available, including:

- ✓ U.S. lead and pulse generator survival probability
- ✓ Worldwide malfunction counts and patterns
- ✓ Worldwide malfunctions during an implant procedure
- ✓ Acute (first month) lead observations
- ✓ Chronic (after first month) lead complications
- ✓ Reasons for out of service
- ✓ Return rates

Your feedback is always welcome, and plays a vital role in our effort to continuously improve our products and services, advancing science to transform the lives of our patients.

Sincerely,

Alexandra Naughton  
Vice President, Quality Assurance

## Boston Scientific Reviewers

**Alexandra Naughton**

Vice President, Quality Assurance

**John Kerrigan**

Senior Director, Quality Assurance

**Maria Macuare-Gorden, M.D.**

Vice President of Medical Safety

**Karla Martinez**

Statistician

**John Risse**

Senior Manager, Product Performance Reporting

## Independent Reviewer

**Professor Douglas Hawkins, Ph.D.**

## Editor

**Steven Brillhart**

Principal Data Analyst

# Statistical Methodology

## What Is Device Survival Probability?

Medical journals have traditionally used patient survival probability to display information on treatment option effectiveness. In the report, **pulse generator and lead** survival probabilities convey information about long-term performance of implantable cardiac rhythm management products.

Device survival probability shows the percentage of implanted devices that remain implanted and in service at various points in a product's service life, in the absence of competing risks, such as natural mortality or voluntary explants. Conceptually, a pulse generator of high reliability and large battery capacity or low current drain remains near 100% survival until eventually, normal battery depletion begins to cause significant numbers of devices to be removed, and the device survival probability drops rapidly. For example, a device survival probability of 99% indicates that within the stated implant duration, the pulse generator had a 1% risk of removal for battery depletion or for incurring a malfunction that required replacement. Survival probabilities are provided with and without normal battery depletions, depicted as "Battery Depletions and Malfunctions" and "Malfunctions Only," respectively.

Boston Scientific estimates survival probability in compliance with the 2014 revision of international standard ISO 5841-2: 2014 (E). Survival probability is calculated at a given time by separately estimating the probability of surviving each interval and multiplying the survival probabilities of all intervals through which a device has passed. To estimate the probability of surviving any interval, the number of units that successfully functioned during the interval is divided by the number of units exposed to malfunction/depletion during the interval. The number of units exposed is calculated using the actuarial method, where device suspensions in an interval are distributed uniformly across the interval. Reasons for device suspension from survival probability statistics are detailed in the report section entitled U.S. Reason for Out of Service.

## Inclusion Criteria for Pulse Generator and Lead Survival Probability Datasets

Pulse generator survival probability is reported for U.S. implanted devices in product families that meet inclusion criteria described below. Lead survival probability is reported for both the U.S. Registered Implant population and for leads enrolled in the Longitude Surveillance Registry, for product families that meet inclusion criteria described below.

To be included in survival probability statistics, a device must first be successfully implanted (defined in this report as occurring upon pocket closure). Prophylactic device removals are tracked as part of the active population up until the time the device is removed from service; devices removed prophylactically and not identified as malfunctions at the time of explant do not contribute to a reduction in survival probability. Reasons for device explant or out of service, if known, are provided in this report for each pulse generator product/product grouping.

Survival probabilities are based on devices registered as implanted in the U.S. Privacy laws in many other geographies preclude manufacturers from obtaining specific patient implant and explant information, thus device survival probabilities cannot be constructed from these data. Boston Scientific considers U.S. experience representative of worldwide performance. The Malfunction Details for leads and pulse generators reflect worldwide malfunctions, inclusive of U.S. data.

Criteria for inclusion of product families in this report are in compliance with the AdvaMed *Industry Guidance for Uniform Reporting of Clinical Performance of Pulse Generators and Leads*. Survival estimates are provided for product families once they have at least 10,000 cumulative U.S. implant

months. The minimum interval sample size is 200 U.S. implanted units. Pulse generator product families with fewer than 500 total remaining estimated active U.S. devices are not included in this report. Lead product families that received original U.S. market release approval twenty or more years ago are not included in this report.

Estimated Longevity information is provided for pulse generator products in the U.S. Survival Probability - Battery Depletions and Malfunctions graphs, depicted as a blue bar on the x axis for Years Implanted. The estimated longevity values from the Instructions for Use for each product family are used to construct the blue longevity bars on their U.S. Survival Probability graph. They represent the range of estimated longevity based on a variety of programmed settings and therapy usage.

Survival probability data are presented in tabular and graphical formats online at [www.bostonscientific.com/ppr](http://www.bostonscientific.com/ppr). Performance data for Intermedics products may also be found on [www.bostonscientific.com/ppr](http://www.bostonscientific.com/ppr). Specific inclusion criteria for pulse generator and lead survival probability datasets are described here. Not all products may be approved for use in all geographies, as product approval is geography specific.

Worldwide distribution, U.S. registered implant, and U.S. estimated active implant numbers have been rounded to provide population size context.

To convey implant experience for a product family, U.S. approval dates are provided. The U.S. approval date listed is the earliest date Boston Scientific received approval for one or more of the models in the family.

### **Survival Probability – Battery Depletions and Malfunctions (Pulse Generators)**

Reduction in survival probability for **pulse generators** is due to:

- Devices removed for normal battery depletion
- Device malfunctions occurring while implanted, as confirmed by returned product analysis

### **Survival Probability – Malfunctions Only (Pulse Generators)**

Reduction in survival probability for **pulse generators** is due only to:

- Device malfunctions occurring while implanted, as confirmed by returned product analysis; premature battery depletions are considered device malfunctions.

In this case, normal battery depletions do not contribute to the reduction in survival probability; rather, reduction in survival probability is due only to confirmed pulse generator malfunctions. Furthermore, unconfirmed reports of premature battery depletions do not reduce “Malfunctions Only” survival probability. Put another way, this information depicts the percentage of confirmed malfunction-free devices remaining in service at various intervals in the product's service life, based on returned product analysis.

### **Survival Probability — Complications and Malfunctions (Leads)**

The 2014 version of ISO 5841-2: 2014(E) outlines a methodology for lead survival probability inclusion. Boston Scientific has applied this methodology for survival probability to all lead families implanted as of May 2009 and forward. Worldwide malfunctions are not included for previous lead families.

Reduction in survival probability is due to:

- Leads and lead segments returned for analysis and determined to be non-compliant in form, fit, or function at any time while implanted
- Leads removed from service with reported complications 30 days or more post-implant, whether returned or not. See the Chronic Lead Complications Table in this report for the observations which are included.

### **Further Adjustments for Device and Lead Survival**

Because underreporting of patient deaths unrelated to device function would result in overestimation of pulse generator or lead survival by overstating the number of devices in service, Boston Scientific addresses this underreporting in two ways. First, regular updates are obtained from the Social Security Administration about deceased persons and compared to Boston Scientific patient data to identify patients who have died but whose deaths had not been reported to Boston Scientific. Second, Boston Scientific uses 10% annual patient mortality as a baseline and adjusts reported patient deaths in any interval for which reports are less than the baseline rate. No adjustment is applied to account for underreporting of malfunctions, as the rate of underreporting is unknown.

Boston Scientific does not make statistical adjustments to account for underreporting of battery depletion. However, as mentioned earlier, Boston Scientific includes non-returned devices removed from service for battery depletion with no associated complaint as normal battery depletions.

### **Categorization of Malfunctions for Survival Probability Reporting**

Malfunctions represent pulse generators and leads removed from service and confirmed through laboratory analysis to have operated outside the specified performance limits established by Boston Scientific while implanted and in service. Device damage occurring during or after explant, or caused by external factors including those warned against in product labeling (such as ionizing therapeutic radiation), are not reported as device malfunctions in survival data. Damage to a pulse generator caused by a lead malfunction is reported as a lead malfunction. Malfunctions are further classified according to their impact on therapy, as follows:

- **Malfunction With Compromised Therapy —**

The condition when a device is confirmed through laboratory analysis to have malfunctioned in a manner that compromised pacing or defibrillation therapy (including complete loss or partial degradation) while implanted and in service.

Examples include (but are not limited to): sudden loss of battery voltage; accelerated current drain such that low battery was not detected before loss of therapy; sudden malfunction during defibrillation therapy resulting in aborted therapy delivery; intermittent malfunction in which therapy is compromised while in the malfunction state.

- **Malfunction Without Compromised Therapy —**

The condition when a device is confirmed through laboratory analysis to have malfunctioned in a manner that did not compromise pacing or defibrillation therapy while implanted and in service. Malfunctions in which critical patient-protective pacing and defibrillation therapies remain available are included here.

Examples include (but are not limited to): error affecting diagnostic functions, telemetry function, data storage; malfunction of a component that causes the battery to lose power quickly enough to result in premature battery depletion, but slowly enough that the condition is detected through normal follow-up before therapy is lost; mechanical problems with connector header that do not affect therapy.

### **Categorization of Normal Battery Depletion for Survival Probability Reporting**

Per the AdvaMed *Industry Guidance for Uniform Reporting of Clinical Performance of Pulse Generators and Leads*, **Normal Battery Depletion** is defined as the condition when:

- a) A device is returned with no associated complaint and the device has reached its elective replacement indicator(s) with implant time that meets or exceeds the nominal (50 percentile) predicted longevity at default (labeled) settings, or
- b) A device is returned and the device has reached its elective replacement indicator(s) with implant time exceeding 75% of the expected longevity using actual device settings and therapeutic use.

Boston Scientific includes within this count both returned *and non-returned* devices removed from service for battery depletion with no associated complaint. In conformance with the AdvaMed guidance document, Boston Scientific performs battery usage analysis, including battery status verification, on all devices returned without a complaint. We continue to include non-returned devices reported by our customers as being removed from service due to normal battery depletion within this count.

### **Boston Scientific CRM's Corrective and Preventive Actions (CAPA) System**

Boston Scientific strives to provide implantable devices of high quality and reliability. However, these devices are not perfect and may exhibit malfunctions at a low rate of occurrence. Device performance information is received from many sources through various channels. Boston Scientific monitors information from many sources including suppliers, testing, manufacturing and field performance to identify opportunities for improvement.

When a device is returned to Boston Scientific, laboratory technicians and engineers assess overall device function and perform analysis using specific tests related to the clinical observation(s). Test results are compared to original manufacturing records and design intent. Clinical observations are added to laboratory findings to help determine cause of the clinical observation(s). Each discrete event is then compared to other similar-appearing events. If a pattern is detected, actions are taken to identify a common root cause, and improvements intended to improve product reliability and/or performance may be implemented. Observations from supplier data and internal manufacturing operations also lead to opportunities for improvement. Improvements, when made, may include design changes, manufacturing and supplier process modifications, software updates, educational communications, or labeling changes to preceding, existing, or subsequent generations. Improvement implementation may vary by geography due to various factors including regulatory review timing. They may not be applied to every product susceptible to the malfunction pattern and may not mitigate or eliminate the potential for additional malfunctions. In cases where an improvement is made to an approved product line, devices made without the improvement may continue to be distributed where such products meet our high reliability and performance standards, particularly when changes are incremental and in accordance with our overall philosophy of continuous product improvement.

Improvements are closely monitored for effectiveness. Boston Scientific informs regulatory bodies of each significant event that poses potential risk to patient health to meet regulatory obligations, and shares returned product investigation findings with physicians. The malfunction details section for pulse generators and leads includes a summary of these findings.

In summary, thorough investigation of internal and external data coupled with low trigger levels for improvements creates a continuous product improvement system that is very responsive to patient and physician needs. Boston Scientific is committed to sharing an accurate picture of product performance and addressing identified opportunities for improvement in a timely fashion for our customers.

# Malfunction Details: Overview

Boston Scientific CRM pursues product quality and reliability with a passion. We therefore continuously monitor product performance to make improvements whenever possible. Worldwide Malfunction tables provide a count and description of malfunctions associated with the majority of actively in-service Boston Scientific products. Intermedics co-branded product data are included in corresponding pacemaker and pacing lead malfunction counts and details. Information presented is based on malfunctions reported to and analyzed by Boston Scientific. Each table contains malfunction counts listed by category, pattern and therapy availability.

## Category

Malfunctions are categorized by the nature of their root cause. For example, a malfunction due to the software within a pulse generator is listed in the Software category. There are four pulse generator malfunction categories and four malfunction categories for leads (described below).

## Patterns

Patients and physicians have asked for more access to Quality System details; therefore, we provide information on patterns of product performance. Patterns listed are informational and do not represent actions that need to be taken. Boston Scientific is committed to direct communication when predicted product performance fails to achieve design or performance expectations or when actions may be taken to improve patient outcomes. Malfunctions associated with product advisories are denoted. Refer to the Product Advisories section for more information. In cases where more than one malfunction pattern could be applied to a device, a single malfunction pattern is reported, with priority given to patterns associated with an advisory, patterns associated with an existing investigation, and malfunctions that resulted in compromised therapy.

Each pattern description includes:

- **Clinical Manifestation and Root Cause** – Malfunctions for each product are characterized according to root cause. Descriptions provide clinical observations and/or analysis findings associated with each malfunction pattern listed in this report. Malfunctions listed within “Other” either do not yet have an identified root cause, or are related to a proprietary product feature, such as connectors or seal rings.
- **Improvement Implementation** – All of the patterns listed are thoroughly investigated and analyzed. As part of Boston Scientific's process of continuous improvement, when possible, improvements have been or will be implemented in response to identified malfunction patterns. Improvements may include product design changes in existing or subsequent generations, manufacturing process modifications, software updates, educational communications or labeling changes. Improvement implementation may vary by geography due to various factors, including regulatory review timing. They may not be applied to every product susceptible to the malfunction pattern, and may not completely mitigate or eliminate the potential for additional malfunctions.

Pattern information in this report is dynamic. Pattern names, superscript number assignments and descriptions may all change from quarter to quarter; as Boston Scientific's investigations progress and improvements are implemented, updated information is provided.

## Therapy Availability

Malfunctions are further classified according to their impact on therapy, as follows:

- **Malfunction With Compromised Therapy** – The condition when a device is confirmed through laboratory analysis to have malfunctioned in a manner that compromised pacing or defibrillation therapy (including complete loss or partial degradation) while implanted and in service. Examples include (but are not limited to): sudden loss of battery voltage; accelerated current drain such that low battery was not detected before loss of therapy; sudden malfunction during defibrillation therapy resulting in aborted therapy delivery; intermittent malfunction in which therapy is compromised while in the malfunction state.
- **Malfunction Without Compromised Therapy** – The condition when a device is confirmed through laboratory analysis to have malfunctioned in a manner that did not compromise pacing or defibrillation therapy while implanted and in service. Malfunctions in which critical patient-protective pacing and defibrillation therapies remain available are included here. Examples include (but are not limited to): error affecting diagnostic functions, telemetry function, data storage; malfunction of a component that causes the battery to lose power quickly enough to result in premature battery depletion, but slowly enough that the condition is detected through normal follow-up before therapy is lost; mechanical problems with connector header that do not affect therapy.

## Pulse Generator Malfunctions

Pulse generator malfunctions represent devices removed from service and confirmed through laboratory analysis to have operated outside the performance limits established by Boston Scientific while implanted and in service. Device damage occurring during or after explant, or caused by external factors including those warned against in product labeling (e.g. therapeutic radiation), are not considered device malfunctions. Damage to a pulse generator caused by a lead malfunction is reported as a lead malfunction.


## Lead Confirmed Malfunctions

Lead confirmed malfunctions represent leads removed from service and confirmed through laboratory analysis to have operated outside the performance limits established by Boston Scientific while implanted and in service. The Boston Scientific Product Performance Report is in compliance with the 2014 version of ISO 5841-2: 2 (E), Reporting of Clinical Performance of Populations of Pulse Generators or Leads. This version categorizes leads with reported complications which are taken out of service and returned, but for which no malfunction can be confirmed, as Chronic Lead Complications. This methodology also addresses the Recommendations from the Heart Rhythm Society Task Force on Lead Performance Policies and Guidelines.

# RESONATE/MOMENTUM/CHARISMA/VIGILANT CRT-D

Models: G124/G125/G126/G128/G138/G224/G225/G228/G237/G247/G248/G324/G325/G347/G348/  
G424/G425/G426/G428/G437/G447/G448/G524/G525/G526/G528/G537/G547/G548

US Summary			
US Registered Implants:	89,000	US Normal Battery Depletions:	255
US Approval Date:	September 2017	US Malfunctions:	50
US Estimated Active Implants:	80,000	Without Compromised Therapy:	38
		With Compromised Therapy:	12

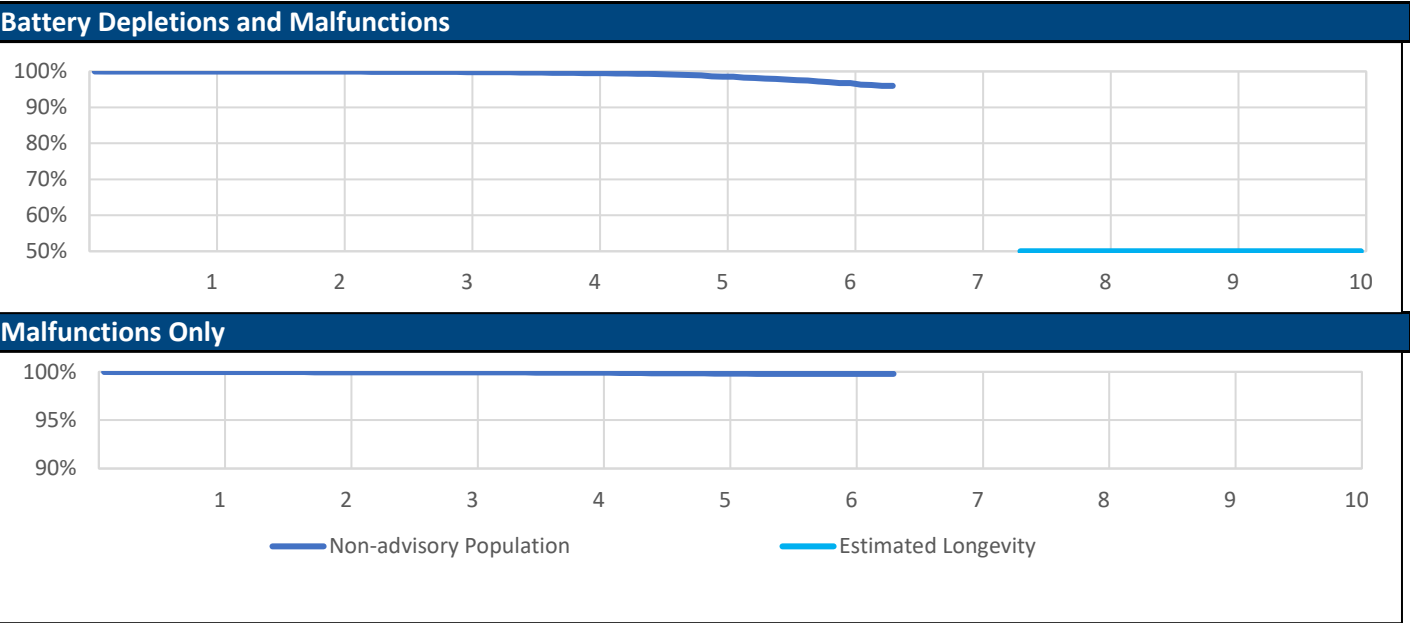

US Survival Probability											
	Year	1	2	3	4	5	6	7	8	9	10
Non-Advisory Population	Depletions and Malfunctions	100.0%	99.9%	99.8%	99.6%	98.7%	96.8%	96.0%	--	--	--
Registered Implants:	Malfunctions Only	100.0%	100.0%	100.0%	99.9%	99.8%	99.8%	99.8%	--	--	--
89,000	Effective Sample Size	64577	44736	29010	16513	7505	1568	287	--	--	--

@ 77 months

# RESONATE/MOMENTUM/CHARISMA/VIGILANT CRT-D

Models: G124/G125/G126/G128/G138/G224/G225/G228/G237/G247/G248/G324/G325/G347/  
G348/G424/G425/G426/G428/G437/G447/G448/G524/G525/G526/G528/G537/G547/G548

Worldwide Confirmed Malfunctions	90
Worldwide Distribution	164,000

US Approval Date: September 2017	With Compromised Therapy	Without Compromised Therapy	Total
Electrical			
Integrated circuit (63)	6	14	20
Low-voltage capacitor (69)	0	14	14
Battery (53)	2	18	20
High voltage capacitor (75)	2	0	2
Software			
Memory errors (51)	1	19	20
Other			
Non-patterned, other	6	8	14
Grand Total	17	73	90

References cited in table above [\(link\)](#)

# AUTOGEN CRT-D

Models: G160/G161/G164/G166/G168/G172/G173/G175/G177/G179


Worldwide Confirmed Malfunctions		40	
Worldwide Distribution		25,000	
US Approval Date: April 2014	With Compromised Therapy	Without Compromised Therapy	Total
Electrical			
High voltage circuit component (62)	0	7	7
Integrated circuit (63)	2	4	6
Low-voltage capacitor (69)	0	6	6
Battery (53)	3	9	12
High voltage capacitor (75)	1	0	1
Software			
Safety Core-unintended biventricular pacing (64)	0	1	1
Memory errors (51)	0	1	1
Other			
Non-patterned, other	1	5	6
Grand Total	7	33	40

References cited in table above [\(link\)](#)

# DYNAGEN/INOGEN/ORIGEN CRT-D

Models: G050/G051/G056/G058/G140/G141/G146/G148/G150/G151/G154/G156/G158

US Summary			
US Registered Implants:	76,000	US Normal Battery Depletions:	3,086
US Approval Date:	April 2014	US Malfunctions:	127
US Estimated Active Implants:	56,000	Without Compromised Therapy:	114
		With Compromised Therapy:	13

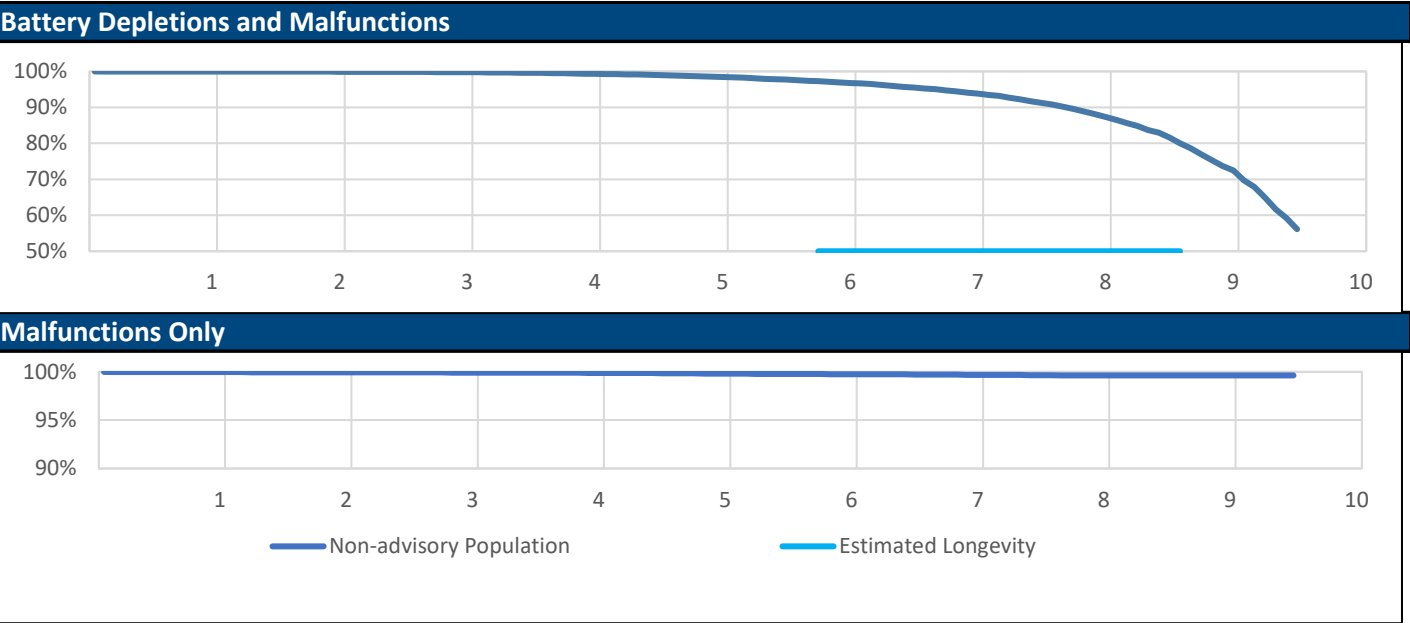

US Survival Probability											
	Year	1	2	3	4	5	6	7	8	9	10
Non-Advisory Population	Depletions and Malfunctions	100.0%	99.9%	99.8%	99.4%	98.6%	97.0%	94.1%	88.1%	73.7%	56.1%
Registered Implants:	Malfunctions Only	100.0%	99.9%	99.9%	99.9%	99.8%	99.8%	99.7%	99.6%	99.6%	99.6%
76,000	Effective Sample Size	65962	57782	49917	42089	34191	25334	15896	7386	1797	241

@ 115 months

# DYNAGEN/INOGEN/ORIGEN CRT-D

Models: G050/G051/G056/G058/G140/G141/G146/G148/G150/G151/G154/G156/G158


Worldwide Confirmed Malfunctions		179	
Worldwide Distribution		136,000	
US Approval Date: April 2014	With Compromised Therapy	Without Compromised Therapy	Total
Electrical			
High voltage circuit component (62)	0	19	19
Integrated circuit (63)	4	11	15
Low-voltage capacitor (69)	0	31	31
High voltage capacitor (75)	2	1	3
Battery (53)	2	40	42
Low-voltage capacitors (47)	0	1	1
Software			
Memory errors (51)	2	35	37
Safety Core-unintended biventricular pacing (64)	0	3	3
Other			
Non-patterned, other	13	15	28
Grand Total	23	156	179

References cited in table above [\(link\)](#)

# INCEPTA/ENERGEN/PUNCTUA CRT-D

Models: N050/N051/N052/N053/N140/N141/N142/N143/N160/N161/N162/N163/N164/N165/P052/P053/P142/P143/P162/P163/P165

US Summary			
US Registered Implants:	53,000	US Normal Battery Depletions:	11,497
US Approval Date:	November 2011	US Malfunctions:	811
US Estimated Active Implants:	18,000	Without Compromised Therapy:	788
		With Compromised Therapy:	23

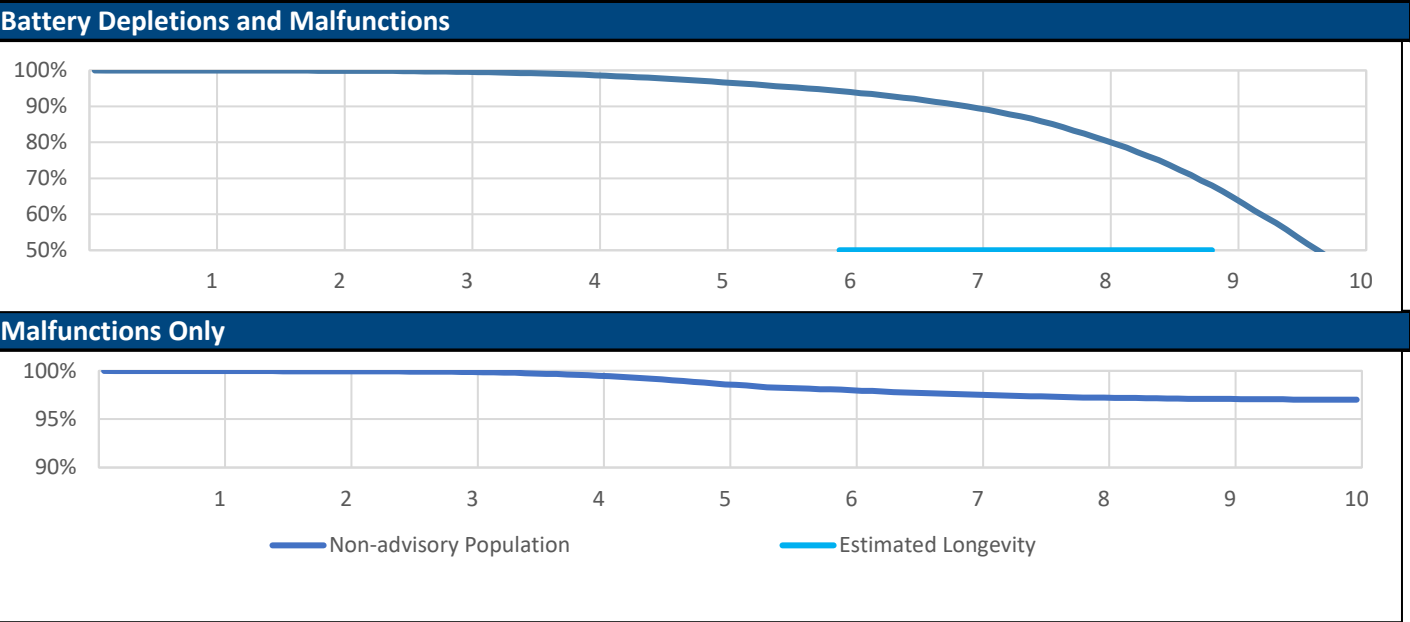

US Survival Probability											
Year		1	2	3	4	5	6	7	8	9	10
Non-Advisory Population Registered Implants: 53,000	Depletions and Malfunctions	100.0%	99.9%	99.6%	98.8%	96.9%	94.3%	90.0%	81.5%	66.4%	44.0%
	Malfunctions Only	100.0%	100.0%	99.9%	99.5%	98.7%	98.0%	97.6%	97.2%	97.1%	97.0%
	Effective Sample Size	46296	41442	36980	32822	28766	24958	21278	17148	11981	5213

# INCEPTA/ENERGEN/PUNCTUA CRT-D

Models: N050/N051/N052/N053/N140/N141/N142/N143/N160/N161/N162/N163/N164/N165/  
P052/P053/P142/P143/P162/P163/P165

Worldwide Confirmed Malfunctions	1,297
Worldwide Distribution	81,000


US Approval Date: November 2011	With Compromised Therapy	Without Compromised Therapy	Total
Electrical			
Safety Core-electrocautery (42)	1	6	7
High-voltage capacitor (43)	5	0	5
Low-voltage capacitors (47)	0	1	1
Integrated circuit (50)	7	2	9
Battery (53)	2	11	13
Low-voltage capacitor (54)	7	1205	1212
Low-voltage capacitor (69)	0	11	11
Mechanical			
Transformer (38)	6	0	6
Software			
Memory errors (51)	0	9	9
Other			
Non-patterned, other	8	16	24
Grand Total	36	1261	1297

References cited in table above [\(link\)](#)

# COGNIS CRT-D

Models: N106/N107/N108/N118/N119/N120/P106/P107/P108

US Summary			
US Registered Implants:	75,000	US Normal Battery Depletions:	15,956
US Approval Date:	March 2008	US Malfunctions:	2,099
US Estimated Active Implants:	14,000	Without Compromised Therapy:	1,906
		With Compromised Therapy:	193

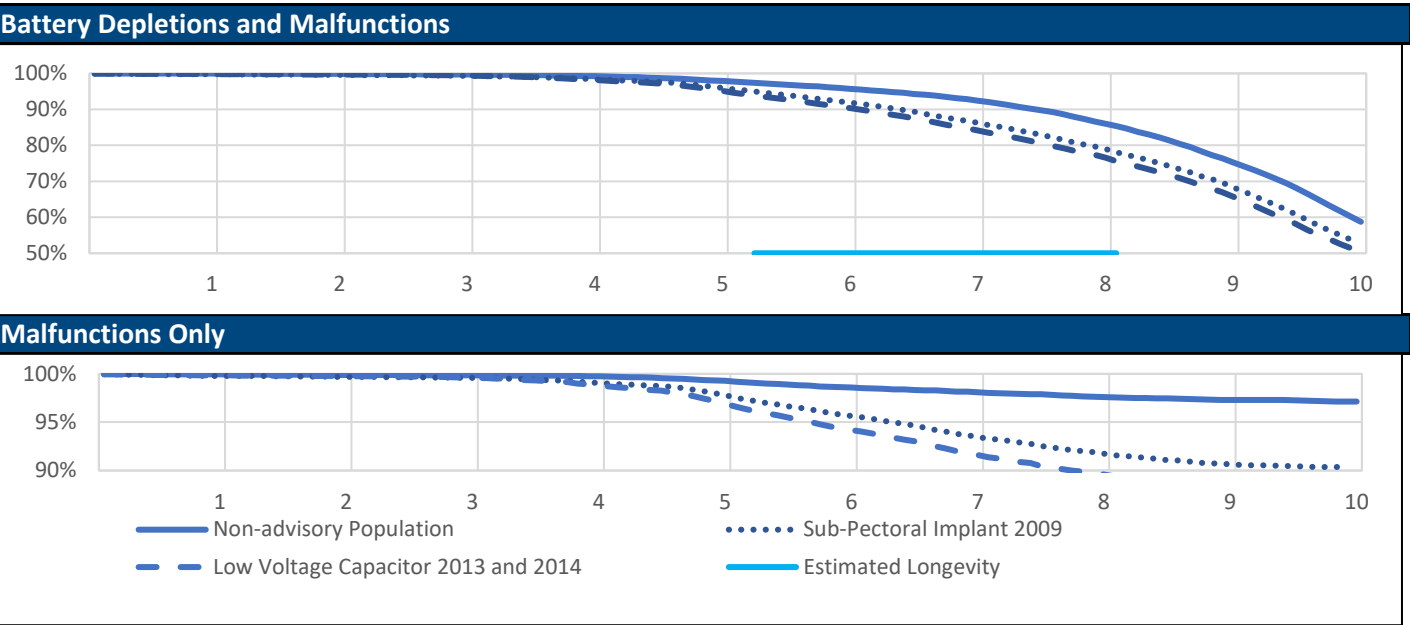

US Survival Probability											
	Year	1	2	3	4	5	6	7	8	9	10
Non-Advisory Population	Depletions and Malfunctions	99.9%	99.8%	99.7%	99.3%	98.0%	96.0%	92.9%	86.6%	76.4%	60.3%
Registered Implants:	Malfunctions Only	99.9%	99.9%	99.9%	99.8%	99.3%	98.6%	98.1%	97.6%	97.3%	97.1%
36,000	Effective Sample Size	31260	28029	25087	22365	19813	17329	14952	12457	9757	6854

# COGNIS CRT-D

Models: N106/N107/N108/N118/N119/N120/P106/P107/P108

US Survival Probability (cont.)											
Year		1	2	3	4	5	6	7	8	9	10
Subpectoral Implant 2009	Depletions and Malfunctions	99.8%	99.6%	99.4%	98.5%	96.3%	92.2%	86.8%	79.6%	69.6%	53.9%
	Malfunctions Only	99.8%	99.7%	99.6%	99.1%	98.0%	95.8%	93.7%	91.9%	90.7%	90.4%
	Effective Sample Size	27323	24210	21612	19181	16748	14271	11952	9723	7531	5139
Low Voltage Capacitor 2013 and 2014	Depletions and Malfunctions	99.8%	99.7%	99.5%	98.4%	95.5%	90.7%	84.7%	77.3%	66.9%	51.5%
	Malfunctions Only	99.8%	99.8%	99.6%	98.9%	97.2%	94.4%	91.8%	89.8%	88.4%	88.0%
	Effective Sample Size	22464	19936	17824	15773	13718	11581	9605	7763	5962	4015

\*Devices subject to an advisory. Refer to the Advisories for more details. Devices may be part of more than one advisory.

# COGNIS CRT-D


Models: N106/N107/N108/N118/N119/N120/P106/P107/P108

Worldwide Confirmed Malfunctions		2,962	
Worldwide Distribution		109,000	
US Approval Date: March 2008	With Compromised Therapy	Without Compromised Therapy	Total
<b>Electrical</b>			
Low Voltage Capacitor 2014 - August 29, 2013 and September 17, 2014 Voluntary Physician Advisory (3)	83	1617	1700
Safety Core-electrocautery (42)	25	54	79
High-voltage capacitor (43)	6	1	7
Low-voltage capacitors (47)	0	7	7
Integrated circuit (50)	21	8	29
High voltage circuit (52)	1	0	1
Battery (53)	10	51	61
Low-voltage capacitor (54)	12	851	863
Low-voltage capacitor (69)	0	2	2
<b>Mechanical</b>			
Transformer (38)	9	0	9
Difficulty securing lead (41)	8	8	16
Header contacts (45)	8	10	18
Subpectoral implant 2009 - December 01, 2009 Voluntary Physician Advisory (6)	48	20	68
Header (74)	25	9	34
<b>Software</b>			
Safety Core-programming (46)	0	1	1
Alert messages not displayed post-EOL (48)	0	2	2
Memory errors (51)	2	15	17
<b>Other</b>			
Non-patterned, other	11	37	48
<b>Grand Total</b>	<b>269</b>	<b>2693</b>	<b>2962</b>

# VISIONIST/VALITUDE

Models: U125/U128/U225/U226/U228

US Summary			
US Registered Implants:	57,000	US Normal Battery Depletions:	770
US Approval Date:	October 2014	US Malfunctions:	176
US Estimated Active Implants:	46,000	Without Compromised Therapy:	164
		With Compromised Therapy:	12

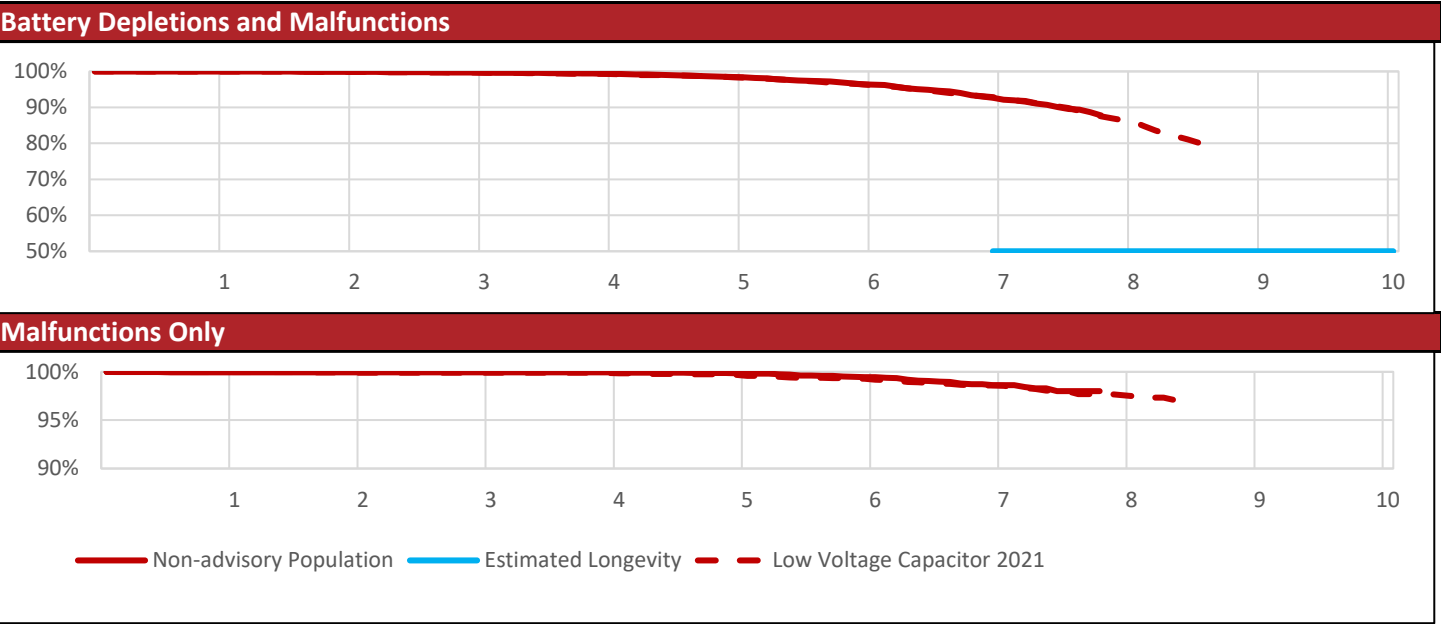

US Survival Probability											
Year		1	2	3	4	5	6	7	8	9	10
Non-Advisory Population	Depletions and Malfunctions	100.0%	99.9%	99.7%	99.4%	98.5%	96.4%	92.6%	87.8%	--	--
Registered Implants:	Malfunctions Only	100.0%	99.9%	99.9%	99.9%	99.9%	99.5%	98.6%	98.0%	--	--
47,000	Effective Sample Size	37671	28142	19887	13728	8589	4541	1588	290	--	--

@ 94 months

\*Devices subject to an advisory. Refer to the Advisories for more details. Devices may be part of more than one advisory.

# VISIONIST/VALITUDE

Models: U125/U128/U225/U226/U228

US Survival Probability (cont.)											
Year		1	2	3	4	5	6	7	8	9	10
Low Voltage Capacitor 2021 Registered Implants: 6,000	Depletions and Malfunctions	100.0%	99.9%	99.7%	99.3%	98.4%	96.4%	92.8%	86.4%	80.2%	--
	Malfunctions Only	100.0%	99.9%	99.9%	99.9%	99.7%	99.3%	98.6%	97.6%	97.1%	--
Effective Sample Size		5915	5283	4717	4199	3699	3127	2386	967	250	--

@ 103 months

\*Devices subject to an advisory. Refer to the Advisories for more details. Devices may be part of more than one advisory.

# VISIONIST/VALITUDE

Models: U125/U128/U225/U226/U228


Worldwide Confirmed Malfunctions		331	
Worldwide Distribution		120,000	
US Approval Date: October 2014	With Compromised Therapy	Without Compromised Therapy	Total
Electrical			
Low-voltage capacitors (47)	0	2	2
Integrated circuit (63)	3	16	19
Telemetry (68)	0	1	1
Hydrogen induced premature depletion - September 2018 (70)	0	20	20
Capacitor (67)	0	1	1
Hydrogen induced premature depletion - June 2021 (83)	2	70	72
High battery impedance (89)	6	150	156
Software			
Memory errors (51)	0	21	21
Other			
Non-patterned, other	9	30	39
Grand Total	20	311	331

References cited in table above [\(link\)](#)

# INTUA/INVIVE/INLIVEN

Models: V272/V273/V282/V283/W272/W273/V172/V173/V182/V183/W172/W173/V274/V275/V284/V285/W275

US Summary			
US Registered Implants:	10,000	US Normal Battery Depletions:	1,249
US Approval Date:	May 2013	US Malfunctions:	588
US Estimated Active Implants:	3,000	Without Compromised Therapy:	565
		With Compromised Therapy:	23

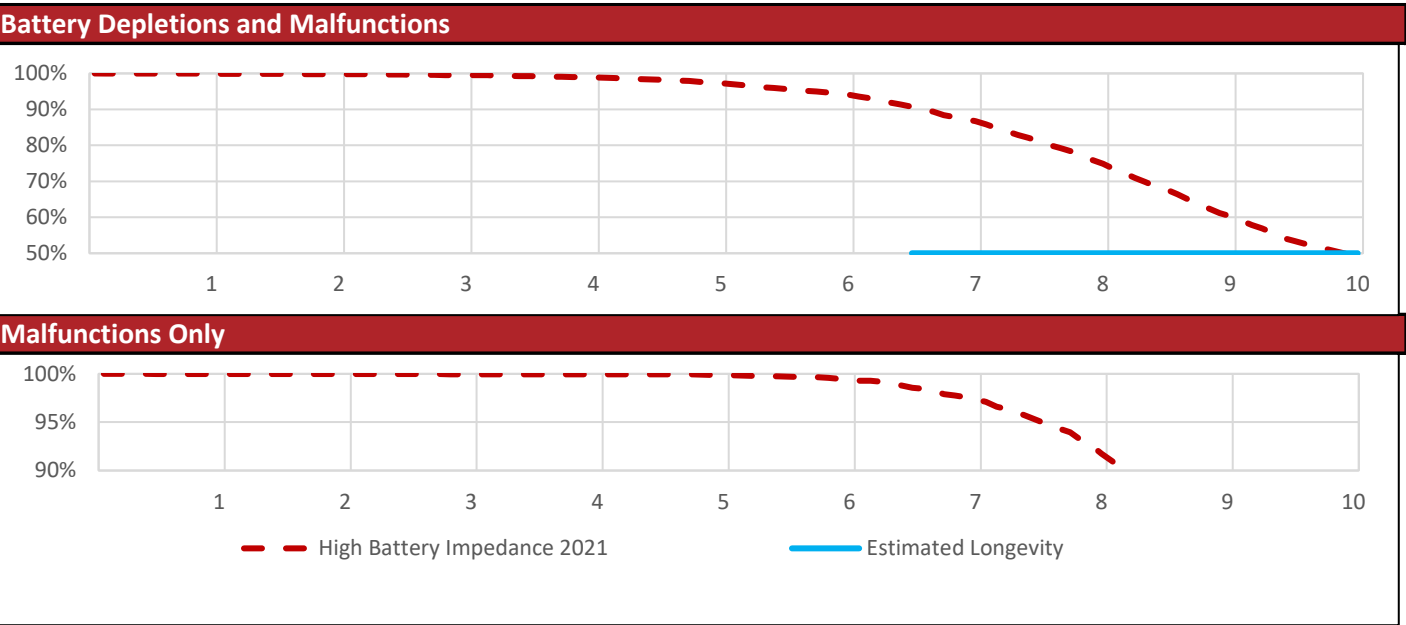

US Survival Probability											
Year		1	2	3	4	5	6	7	8	9	10
High Battery Impedance 2021	Depletions and Malfunctions	99.9%	99.8%	99.5%	99.0%	97.5%	94.3%	87.3%	75.9%	61.2%	49.8%
Registered Implants:	Malfunctions Only	100.0%	100.0%	100.0%	100.0%	99.9%	99.5%	97.6%	92.6%	83.8%	77.5%
10,000	Effective Sample Size	8965	7991	7108	6300	5552	4764	3787	2754	1593	676

\*Devices subject to an advisory. Refer to the Advisories for more details. Devices may be part of more than one advisory.

# INTUA/INVIVE/INLIVEN

Models: V272/V273/V282/V283/W272/W273/V172/V173/V182/V183/W172/W173/V274/V275/V284/V285/W275


Worldwide Confirmed Malfunctions		890	
Worldwide Distribution		24,000	
US Approval Date: May 2013	With Compromised Therapy	Without Compromised Therapy	Total
Electrical			
High battery impedance initiating safety mode 2021 (82)	16	775	791
Low-voltage capacitors (47)	1	0	1
Other			
Non-patterned, other	34	64	98
Grand Total	51	839	890

References cited in table above [\(link\)](#)

# RESONATE/MOMENTUM/CHARISMA/VIGILANT ICD DR

Models: D121/D221/D233/D321/D333/D421/D433/D521/D533

US Summary			
US Registered Implants:	58,000	US Normal Battery Depletions:	39
US Approval Date:	July 2017	US Malfunctions:	23
US Estimated Active Implants:	53,000	Without Compromised Therapy:	16
		With Compromised Therapy:	7

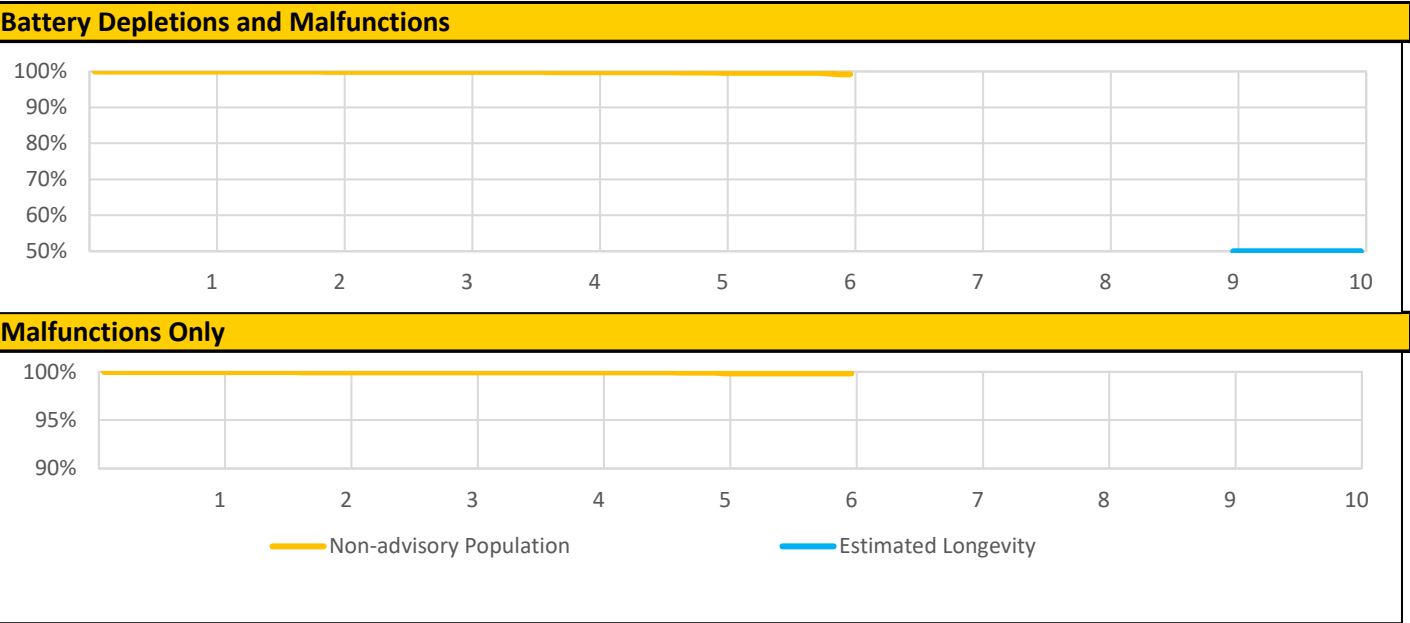

US Survival Probability											
	Year	1	2	3	4	5	6	7	8	9	10
Non-Advisory Population	Depletions and Malfunctions	99.9%	99.9%	99.9%	99.8%	99.7%	99.2%	99.2%	--	--	--
Registered Implants:	Malfunctions Only	100.0%	100.0%	100.0%	99.9%	99.9%	99.8%	99.8%	--	--	--
58,000	Effective Sample Size	39730	25988	15370	7607	2897	419	293	--	--	--

@ 73 months

# RESONATE/MOMENTUM/CHARISMA/VIGILANT ICD DR

Models: D121/D221/D233/D321/D333/D421/D433/D521/D533


Worldwide Confirmed Malfunctions		44	
Worldwide Distribution		106,000	
US Approval Date: July 2017	With Compromised Therapy	Without Compromised Therapy	Total
Electrical			
High voltage capacitor (75)	2	0	2
Integrated circuit (63)	3	6	9
Low-voltage capacitor (69)	0	4	4
Battery (53)	0	8	8
Software			
Memory errors (51)	1	13	14
Mechanical			
Solder joint (88)	1	0	1
Other			
Non-patterned, other	2	4	6
Grand Total	9	35	44

References cited in table above [\(link\)](#)

# RESONATE/MOMENTUM/CHARISMA/VIGILANT ICD VR

Models: D120/D220/D232/D320/D332/D420/D432/D520/D532

US Summary			
US Registered Implants:	32,000	US Normal Battery Depletions:	16
US Approval Date:	July 2017	US Malfunctions:	18
US Estimated Active Implants:	29,000	Without Compromised Therapy:	16
		With Compromised Therapy:	2

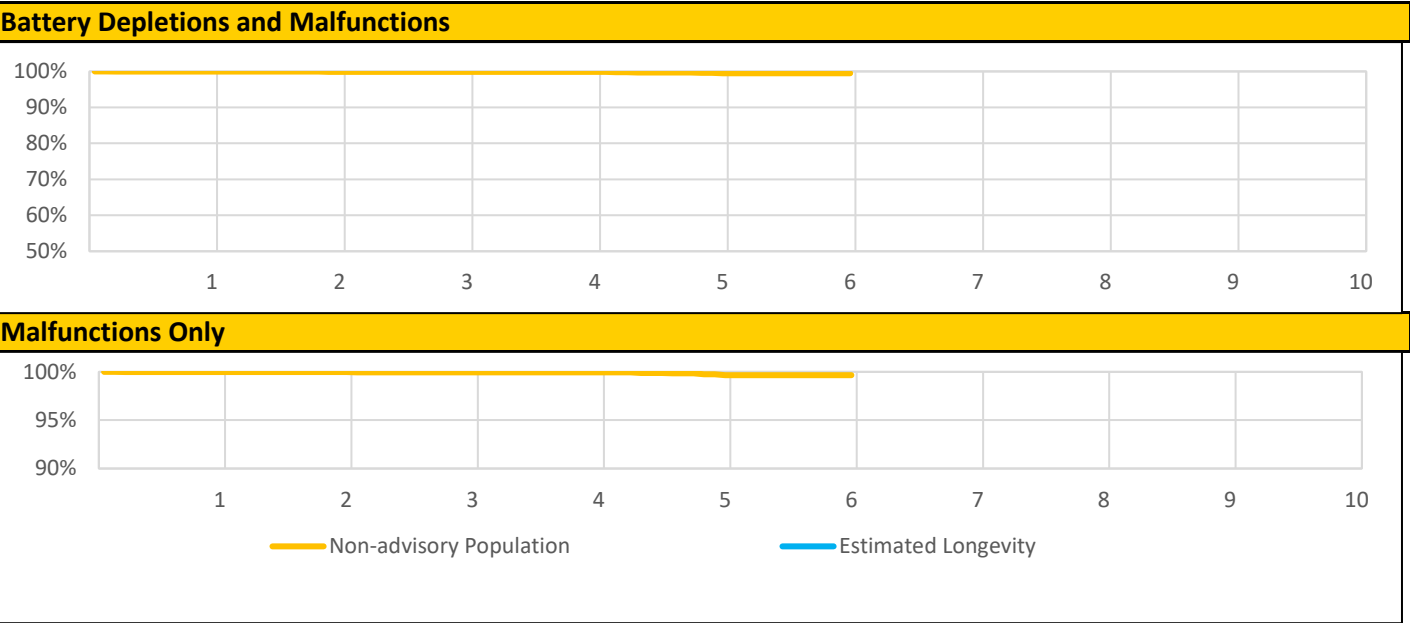

Note: Minimum estimated longevity exceeds 10 years.

US Survival Probability											
	Year	1	2	3	4	5	6	7	8	9	10
Non-Advisory Population	Depletions and Malfunctions	100.0%	99.9%	99.9%	99.8%	99.6%	99.5%	99.5%	--	--	--
Registered Implants:	Malfunctions Only	100.0%	100.0%	100.0%	99.9%	99.8%	99.7%	99.7%	--	--	--
32,000	Effective Sample Size	22035	14462	9120	4979	2097	319	235	--	--	--

@ 73 months

# RESONATE/MOMENTUM/CHARISMA/VIGILANT ICD VR

Models: D120/D220/D232/D320/D332/D420/D432/D520/D532

Worldwide Confirmed Malfunctions		23	
Worldwide Distribution		77,000	
US Approval Date: July 2017	With Compromised Therapy	Without Compromised Therapy	Total
Electrical			
High voltage capacitor (75)	2	0	2
Integrated circuit (63)	1	0	1
Low-voltage capacitor (69)	0	2	2
Low-voltage capacitors (47)	0	1	1
Battery (53)	0	3	3
Software			
Memory errors (51)	0	7	7
Other			
Non-patterned, other	1	6	7
Grand Total	4	19	23

References cited in table above [\(link\)](#)

# PERCIVA DR

Models: D401/D413/D501/D513

US Summary			
US Registered Implants:	5,000	US Normal Battery Depletions:	40
US Approval Date:	July 2017	US Malfunctions:	2
US Estimated Active Implants:	5,000	Without Compromised Therapy:	2
		With Compromised Therapy:	-



US Survival Probability											
Year		1	2	3	4	5	6	7	8	9	10
Non-Advisory Population Registered Implants: 5,000	Depletions and Malfunctions	100.0%	99.9%	99.8%	99.3%	98.1%	96.6%	--	--	--	--
	Malfunctions Only	100.0%	100.0%	99.9%	99.8%	99.8%	99.8%	--	--	--	--
	Effective Sample Size	3997	2734	1627	815	307	215	--	--	--	--

@ 63 months

# PERCIVA DR

Models: D401/D413/D501/D513


Worldwide Confirmed Malfunctions		2	
Worldwide Distribution		10,000	
US Approval Date: July 2017	With Compromised Therapy	Without Compromised Therapy	Total
Other			
Non-patterned, other	0	0	0
Electrical			
Battery (53)	0	1	1
Software			
Memory errors (51)	0	1	1
Grand Total	0	2	2

References cited in table above [\(link\)](#)

# PERCIVA VR

Models: D400/D412/D500/D512

US Summary			
US Registered Implants:	4,000	US Normal Battery Depletions:	8
US Approval Date:	July 2017	US Malfunctions:	3
US Estimated Active Implants:	4,000	Without Compromised Therapy:	2
		With Compromised Therapy:	1

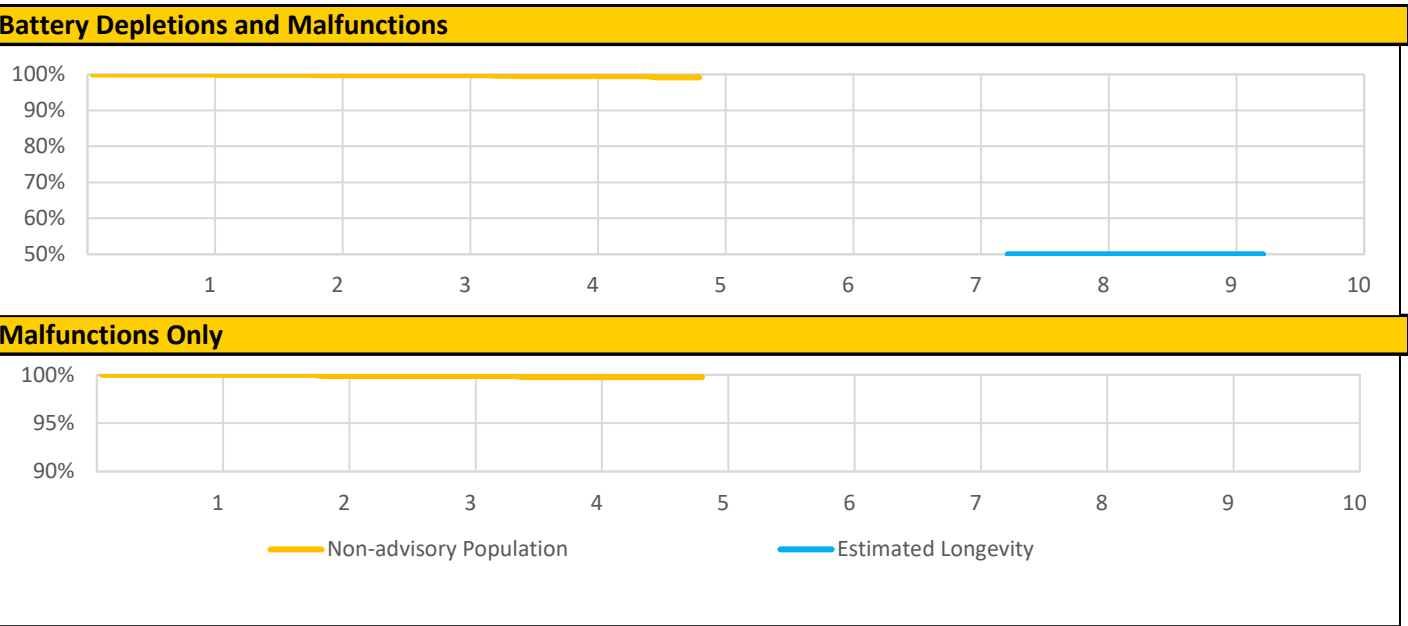

US Survival Probability											
Year		1	2	3	4	5	6	7	8	9	10
Non-Advisory Population	Depletions and Malfunctions	99.9%	99.7%	99.7%	99.5%	99.2%	--	--	--	--	--
	Malfunctions Only	100.0%	99.9%	99.9%	99.8%	99.8%	--	--	--	--	--
	4,000 Effective Sample Size	2851	1783	1049	548	210	--	--	--	--	--

@ 59 months

# PERCIVA VR

Models: D400/D412/D500/D512


Worldwide Confirmed Malfunctions		4	
Worldwide Distribution		7,000	
US Approval Date: July 2017	With Compromised Therapy	Without Compromised Therapy	Total
Software			
Memory errors (51)	0	2	2
Electrical			
Integrated circuit (63)	1	0	1
High voltage capacitor (75)	1	0	1
Grand Total	2	2	4

References cited in table above [\(link\)](#)

# EMBLEM S-ICD

Models: A209/A219

US Summary			
US Registered Implants:	64,000	US Normal Battery Depletions:	1,428
US Approval Date:	March 2015	US Malfunctions:	4,867
US Estimated Active Implants:	49,000	Without Compromised Therapy:	4,703
		With Compromised Therapy:	164

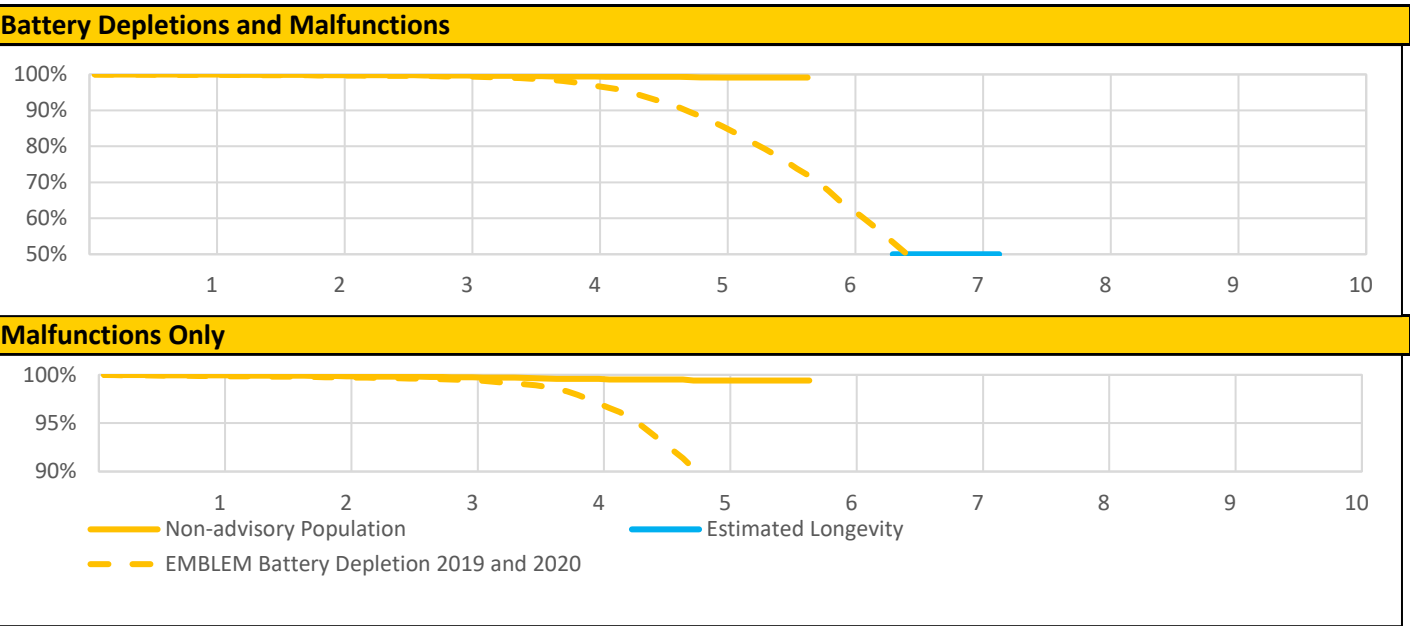

US Survival Probability											
Year		1	2	3	4	5	6	7	8	9	10
Non-Advisory Population Registered Implants: 32,000	Depletions and Malfunctions	99.9%	99.8%	99.7%	99.4%	99.2%	99.1%	--	--	--	--
	Malfunctions Only	99.9%	99.9%	99.7%	99.6%	99.4%	99.4%	--	--	--	--
	Effective Sample Size	30292	20355	12431	6691	2588	208	--	--	--	--

@ 69 months

\*Devices subject to an advisory. Refer to the Advisories for more details. Devices may be part of more than one advisory.

# EMBLEM S-ICD

Models: A209/A219

US Survival Probability (cont.)											
Year		1	2	3	4	5	6	7	8	9	10
Battery Depletion 2019 and 2020 Registered Implants: 22,000	Depletions and Malfunctions	99.9%	99.7%	99.4%	97.4%	87.0%	64.9%	37.7%	18.1%	10.4%	--
	Malfunctions Only	99.9%	99.8%	99.5%	97.5%	88.1%	69.3%	47.0%	31.3%	27.3%	--
	Effective Sample Size	18530	16448	14581	12707	10037	5812	1427	553	246	--

@ 103 months

\*Devices subject to an advisory. Refer to the Advisories for more details. Devices may be part of more than one advisory.

# EMBLEM S-ICD

Models: A209/A219

Worldwide Confirmed Malfunctions		9,927	
Worldwide Distribution		148,000	
US Approval Date: March 2015	With Compromised Therapy	Without Compromised Therapy	Total
Electrical			
High-voltage capacitor (43)	4	0	4
Capacitor (72)	0	1	1
S-ICD battery depletion 2019 and 2020 (77)	151	9406	9557
Battery depletion (84)	1	2	3
Software			
Memory corruption (65)	1	0	1
Misaligned markers (73)	1	3	4
Memory corruption (85)	4	13	17
Mechanical			
Solder joint (78)	13	1	14
EMBLEM S-ICD electrical overstress 2020 (80)	8	0	8
RF antenna (81)	1	0	1
Cracked case (86)	19	1	20
Header (87)	1	0	1
Other			
Non-patterned, other	47	198	245
Telemetry (56)	18	33	51
Grand Total	269	9658	9927

References cited in table above [\(link\)](#)

# AUTOGEN ICD EL DR

Models: D162/D163/D176/D177

Worldwide Confirmed Malfunctions		66	
Worldwide Distribution		16,000	
US Approval Date: April 2014	With Compromised Therapy	Without Compromised Therapy	Total
Electrical			
High voltage circuit component (62)	0	4	4
Integrated circuit (63)	2	0	2
Low-voltage capacitor (69)	0	19	19
Battery (53)	0	29	29
High voltage capacitor (75)	2	0	2
Software			
Memory errors (51)	0	6	6
Other			
Non-patterned, other	1	3	4
Grand Total	5	61	66

References cited in table above [\(link\)](#)

# AUTOGEN ICD EL VR

Models: D160/D161/D174/D175


Worldwide Confirmed Malfunctions		54	
Worldwide Distribution		17,000	
US Approval Date: April 2014	With Compromised Therapy	Without Compromised Therapy	Total
Electrical			
High voltage capacitor (75)	2	0	2
Low-voltage capacitor (69)	0	9	9
Battery (53)	5	31	36
Integrated circuit (63)	0	1	1
Software			
Memory errors (51)	2	2	4
Other			
Non-patterned, other	0	2	2
Grand Total	9	45	54

References cited in table above [\(link\)](#)

# DYNAGEN/INOGEN/ORIGEN ICD EL DR

Models: D052/D053/D142/D143/D152/D153

US Summary			
US Registered Implants:	50,000	US Normal Battery Depletions:	119
US Approval Date:	April 2014	US Malfunctions:	114
US Estimated Active Implants:	40,000	Without Compromised Therapy:	95
		With Compromised Therapy:	19

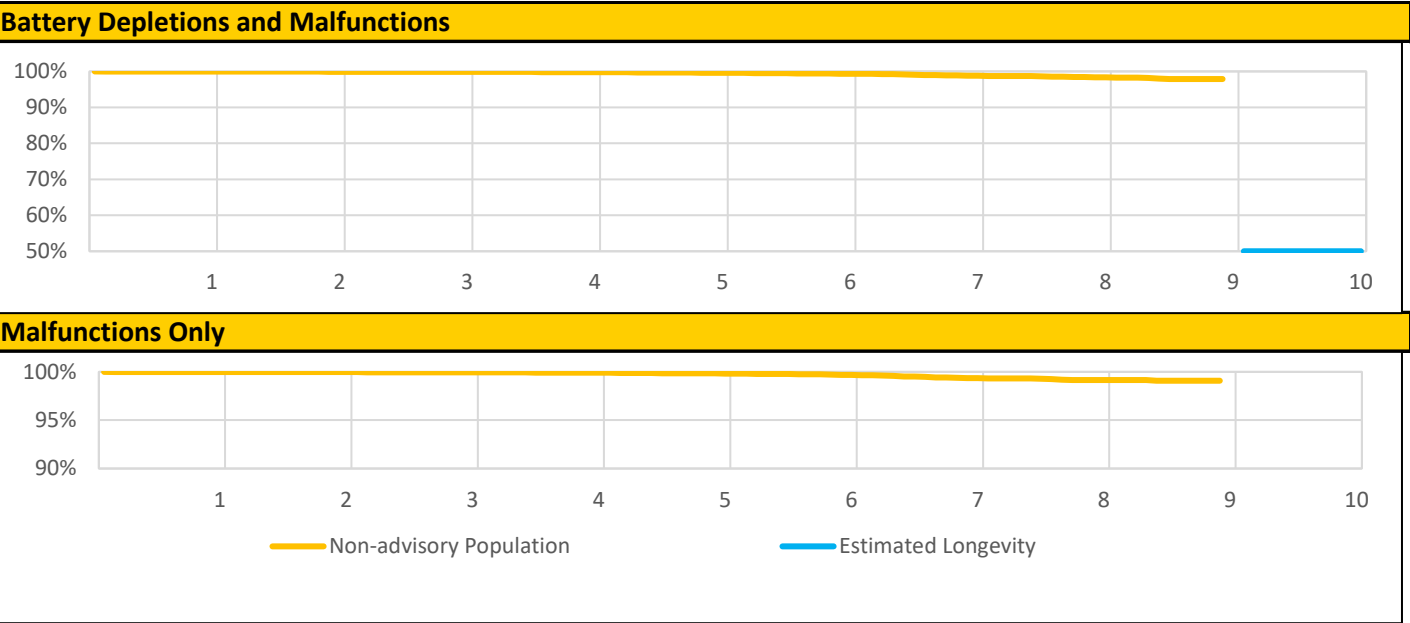

US Survival Probability											
Year		1	2	3	4	5	6	7	8	9	10
Non-Advisory Population Registered Implants:	Depletions and Malfunctions	100.0%	99.9%	99.9%	99.8%	99.6%	99.4%	98.8%	98.4%	97.9%	--
	Malfunctions Only	100.0%	100.0%	99.9%	99.9%	99.8%	99.7%	99.4%	99.1%	99.1%	--
	50,000 Effective Sample Size	43024	36581	30538	24657	19294	13426	7521	3054	319	--

@ 108 months

# DYNAGEN/INOGEN/ORIGEN ICD EL DR

Models: D052/D053/D142/D143/D152/D153


Worldwide Confirmed Malfunctions		145	
Worldwide Distribution		86,000	
US Approval Date: April 2014	With Compromised Therapy	Without Compromised Therapy	Total
Electrical			
Low-voltage capacitors (47)	0	2	2
High voltage circuit component (62)	0	4	4
Integrated circuit (63)	4	1	5
Low-voltage capacitor (69)	0	41	41
High voltage capacitor (75)	8	0	8
Battery (53)	7	56	63
Software			
Memory errors (51)	0	2	2
Other			
Non-patterned, other	8	12	20
Grand Total	27	118	145

References cited in table above [\(link\)](#)

# DYNAGEN/INOGEN/ORIGEN ICD EL VR

Models: D050/D051/D140/D141/D150/D151

US Summary			
US Registered Implants:	39,000	US Normal Battery Depletions:	60
US Approval Date:	April 2014	US Malfunctions:	104
US Estimated Active Implants:	31,000	Without Compromised Therapy:	93
		With Compromised Therapy:	11

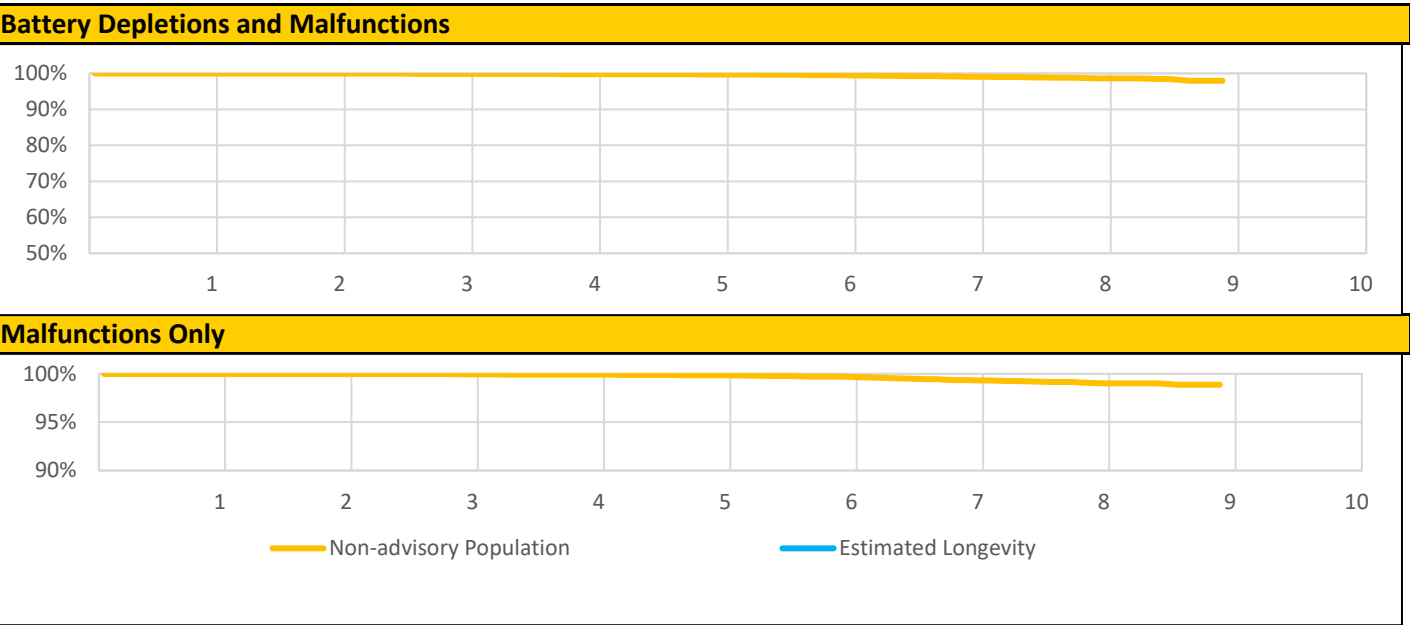

Note: Minimum estimated longevity exceeds 10 years.

US Survival Probability											
	Year	1	2	3	4	5	6	7	8	9	10
Non-Advisory Population Registered Implants:	Depletions and Malfunctions	100.0%	99.9%	99.9%	99.8%	99.7%	99.5%	99.1%	98.7%	97.9%	--
	Malfunctions Only	100.0%	100.0%	100.0%	99.9%	99.9%	99.7%	99.3%	99.1%	98.9%	--
	39,000 Effective Sample Size	33622	28988	24706	20550	16397	11814	6951	3120	282	--

@ 108 months

# DYNAGEN/INOGEN/ORIGEN ICD EL VR

Models: D050/D051/D140/D141/D150/D151


Worldwide Confirmed Malfunctions		149	
Worldwide Distribution		76,000	
US Approval Date: April 2014	With Compromised Therapy	Without Compromised Therapy	Total
Electrical			
Low-voltage capacitors (47)	0	1	1
High voltage circuit component (62)	0	2	2
Integrated circuit (63)	1	2	3
Low-voltage capacitor (69)	1	45	46
Battery (53)	9	58	67
High voltage capacitor (75)	1	0	1
Software			
Memory errors (51)	2	9	11
Other			
Non-patterned, other	6	12	18
Grand Total	20	129	149

References cited in table above [\(link\)](#)

# DYNAGEN/INOGEN/ORIGEN ICD MINI DR

Models: D002/D003/D012/D013/D022/D023

US Summary			
US Registered Implants:	11,000	US Normal Battery Depletions:	2,395
US Approval Date:	April 2014	US Malfunctions:	22
US Estimated Active Implants:	6,000	Without Compromised Therapy:	19
		With Compromised Therapy:	3

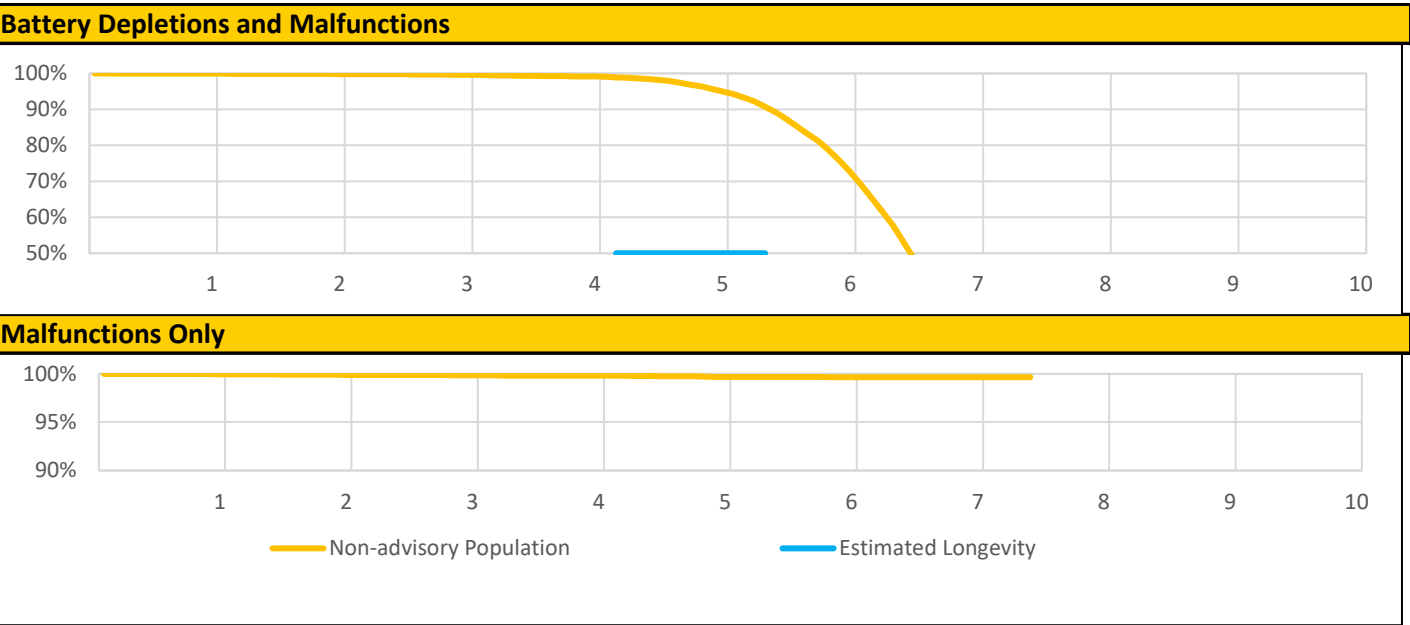

US Survival Probability											
Year		1	2	3	4	5	6	7	8	9	10
Non-Advisory Population Registered Implants:	Depletions and Malfunctions	99.9%	99.9%	99.6%	99.2%	95.7%	75.8%	28.6%	15.1%	--	--
	Malfunctions Only	100.0%	99.9%	99.9%	99.8%	99.7%	99.7%	99.7%	99.7%	--	--
	11,000 Effective Sample Size	9647	8200	6857	5601	4365	2586	631	217	--	--

@ 91 months

# DYNAGEN/INOGEN/ORIGEN ICD MINI DR

Models: D002/D003/D012/D013/D022/D023


Worldwide Confirmed Malfunctions		35	
Worldwide Distribution		34,000	
US Approval Date: April 2014	With Compromised Therapy	Without Compromised Therapy	Total
Electrical			
High voltage circuit component (62)	0	12	12
High voltage capacitor (75)	3	0	3
Integrated circuit (63)	0	2	2
Low-voltage capacitors (47)	1	0	1
Battery (53)	0	4	4
Low-voltage capacitor (69)	0	4	4
Other			
Non-patterned, other	3	6	9
Grand Total	7	28	35

References cited in table above [\(link\)](#)

# DYNAGEN/INOGEN/ORIGEN ICD MINI VR

Models: D000/D001/D010/D011/D020/D021

US Summary			
US Registered Implants:	10,000	US Normal Battery Depletions:	1,534
US Approval Date:	April 2014	US Malfunctions:	18
US Estimated Active Implants:	6,000	Without Compromised Therapy:	17
		With Compromised Therapy:	1

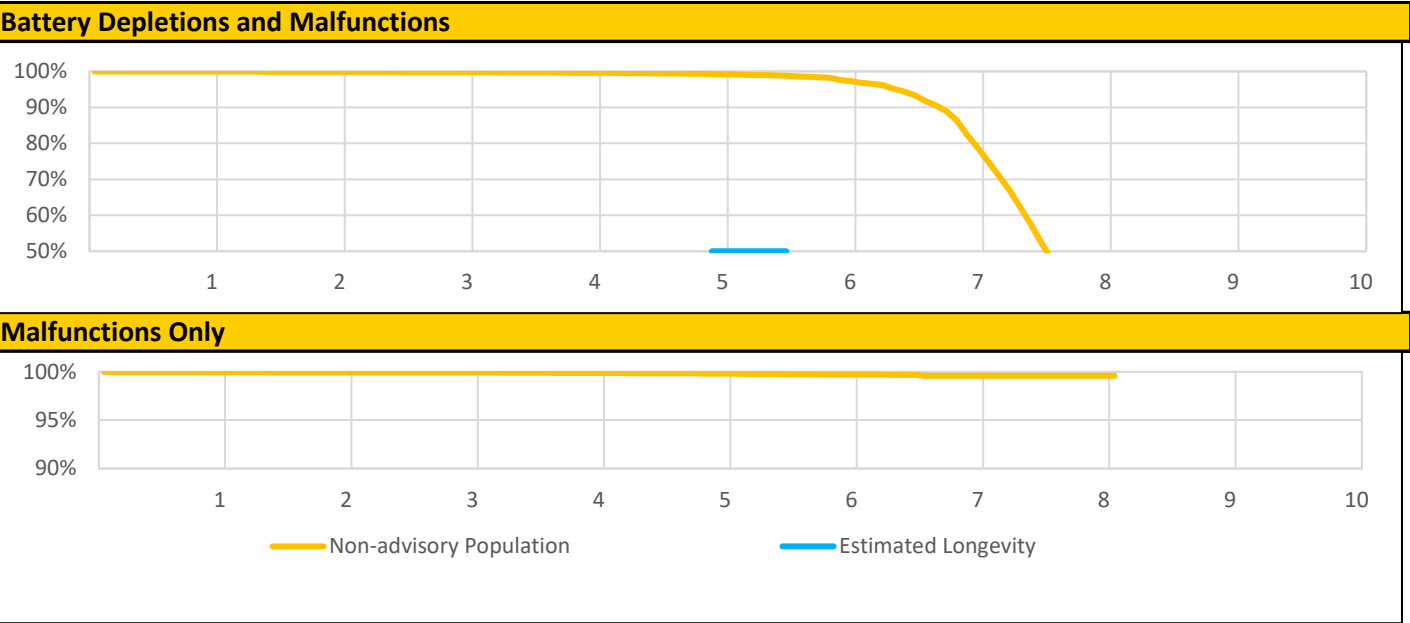

US Survival Probability											
Year		1	2	3	4	5	6	7	8	9	10
Non-Advisory Population Registered Implants:	Depletions and Malfunctions	99.9%	99.9%	99.8%	99.6%	99.2%	97.6%	82.4%	28.0%	19.9%	--
	Malfunctions Only	100.0%	100.0%	99.9%	99.9%	99.8%	99.7%	99.6%	99.6%	99.6%	--
	10,000 Effective Sample Size	8232	7098	6090	5185	4235	3227	1980	406	245	--

@ 99 months

# DYNAGEN/INOGEN/ORIGEN ICD MINI VR

Models: D000/D001/D010/D011/D020/D021


Worldwide Confirmed Malfunctions		39	
Worldwide Distribution		35,000	
US Approval Date: April 2014	With Compromised Therapy	Without Compromised Therapy	Total
Electrical			
Low-voltage capacitors (47)	0	2	2
High voltage circuit component (62)	0	7	7
High voltage capacitor (75)	7	0	7
Low-voltage capacitor (69)	0	6	6
Battery (53)	1	8	9
Software			
Memory errors (51)	1	2	3
Other			
Non-patterned, other	2	3	5
Grand Total	11	28	39

References cited in table above [\(link\)](#)

# INCEPTA/ENERGEN/PUNCTUA ICD DR

Models: E052/E053/E142/E143/E162/E163/F052/F053/F142/F143/F162/F163

US Summary			
US Registered Implants:	47,000	US Normal Battery Depletions:	2,989
US Approval Date:	November 2011	US Malfunctions:	1,295
US Estimated Active Implants:	24,000	Without Compromised Therapy:	1,260
		With Compromised Therapy:	35

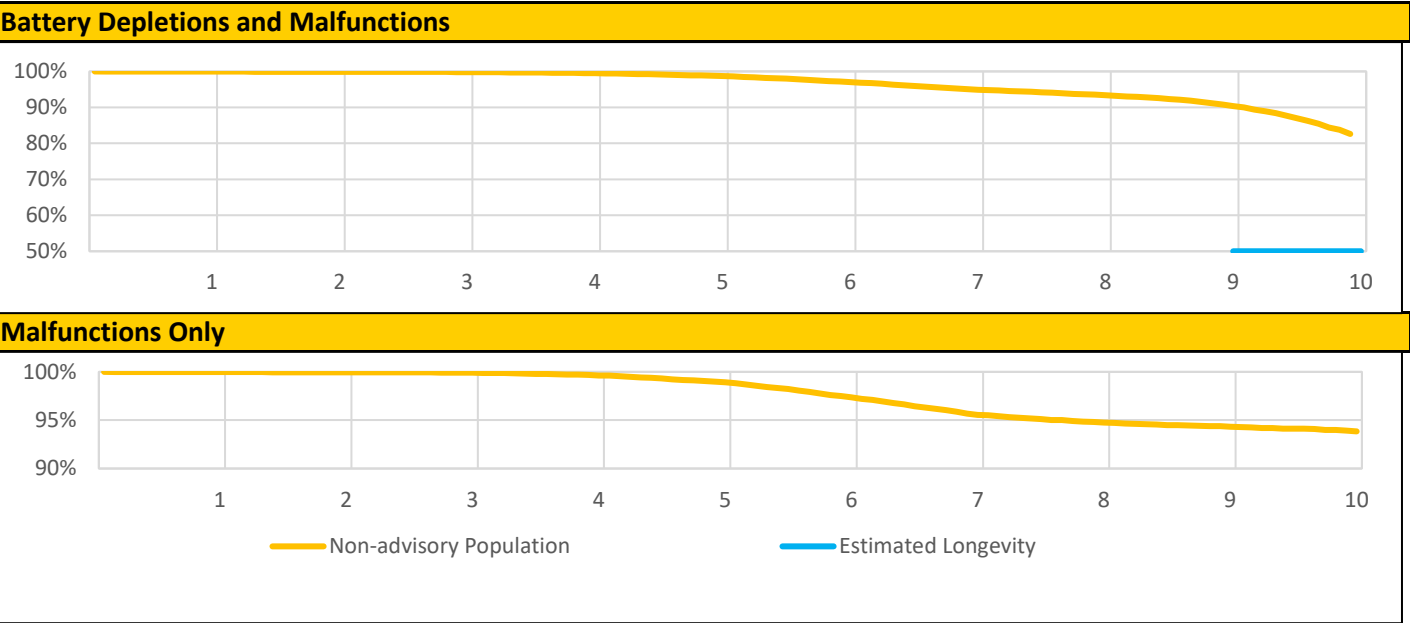

US Survival Probability											
Year		1	2	3	4	5	6	7	8	9	10
Non-Advisory Population	Depletions and Malfunctions	99.9%	99.9%	99.8%	99.5%	98.8%	97.2%	95.1%	93.5%	90.8%	82.6%
	Malfunctions Only	100.0%	100.0%	99.9%	99.7%	99.0%	97.5%	95.7%	94.8%	94.4%	93.9%
	Effective Sample Size	41208	36518	32270	28395	24861	21489	18462	15776	12866	7148

# INCEPTA/ENERGEN/PUNCTUA ICD DR

Models: E052/E053/E142/E143/E162/E163/F052/F053/F142/F143/F162/F163


Worldwide Confirmed Malfunctions		2,007	
Worldwide Distribution		72,000	
US Approval Date: November 2011	With Compromised Therapy	Without Compromised Therapy	Total
Mechanical			
Transformer (38)	2	0	2
Electrical			
High-voltage capacitor (43)	5	1	6
Low-voltage capacitors (47)	0	5	5
Integrated circuit (50)	6	7	13
Battery (53)	15	92	107
Low-voltage capacitor (54)	14	1786	1800
High voltage circuit (58)	0	1	1
Low-voltage capacitor (69)	0	37	37
Software			
Memory errors (51)	0	9	9
Other			
Non-patterned, other	10	17	27
Grand Total	52	1955	2007

References cited in table above [\(link\)](#)

# INCEPTA/ENERGEN/PUNCTUA ICD VR

Models: E050/E051/E140/E141/E160/E161/F050/F051/F140/F141/F160/F161

US Summary			
US Registered Implants:	39,000	US Normal Battery Depletions:	636
US Approval Date:	November 2011	US Malfunctions:	1,323
US Estimated Active Implants:	23,000	Without Compromised Therapy:	1,280
		With Compromised Therapy:	43

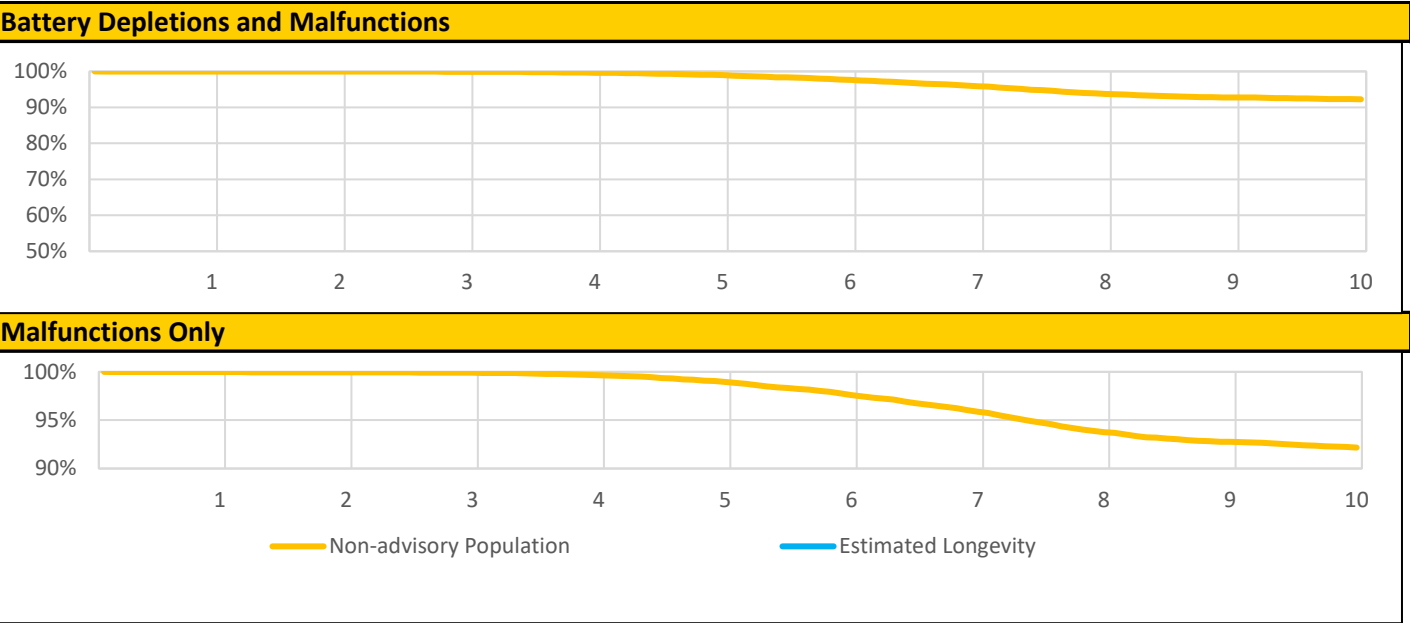

Note: Minimum estimated longevity exceeds 10 years.

US Survival Probability											
Year		1	2	3	4	5	6	7	8	9	10
Non-Advisory Population	Depletions and Malfunctions	100.0%	100.0%	99.9%	99.7%	99.0%	97.8%	96.1%	93.9%	92.8%	92.3%
Registered Implants:	Malfunctions Only	100.0%	100.0%	99.9%	99.7%	99.0%	97.8%	96.1%	93.9%	92.8%	92.2%
39,000	Effective Sample Size	34685	30707	27129	23880	20892	18123	15524	13154	10781	6332

# INCEPTA/ENERGEN/PUNCTUA ICD VR

Models: E050/E051/E140/E141/E160/E161/F050/F051/F140/F141/F160/F161


Worldwide Confirmed Malfunctions		2,223	
Worldwide Distribution		68,000	
US Approval Date: November 2011	With Compromised Therapy	Without Compromised Therapy	Total
Electrical			
High-voltage capacitor (43)	4	1	5
Integrated circuit (50)	5	4	9
Battery (53)	27	152	179
Low-voltage capacitor (54)	19	1938	1957
High voltage circuit (58)	1	0	1
Low-voltage capacitor (69)	0	28	28
Mechanical			
Transformer (38)	6	0	6
Software			
Memory errors (51)	1	9	10
Other			
Non-patterned, other	11	17	28
Grand Total	74	2149	2223

References cited in table above [\(link\)](#)

# SQ-RX S-ICD

Models: 1010

US Summary			
US Registered Implants:	8,000	US Normal Battery Depletions:	2,986
US Approval Date:	September 2012	US Malfunctions:	117
US Estimated Active Implants:	2,000	Without Compromised Therapy:	49
		With Compromised Therapy:	68

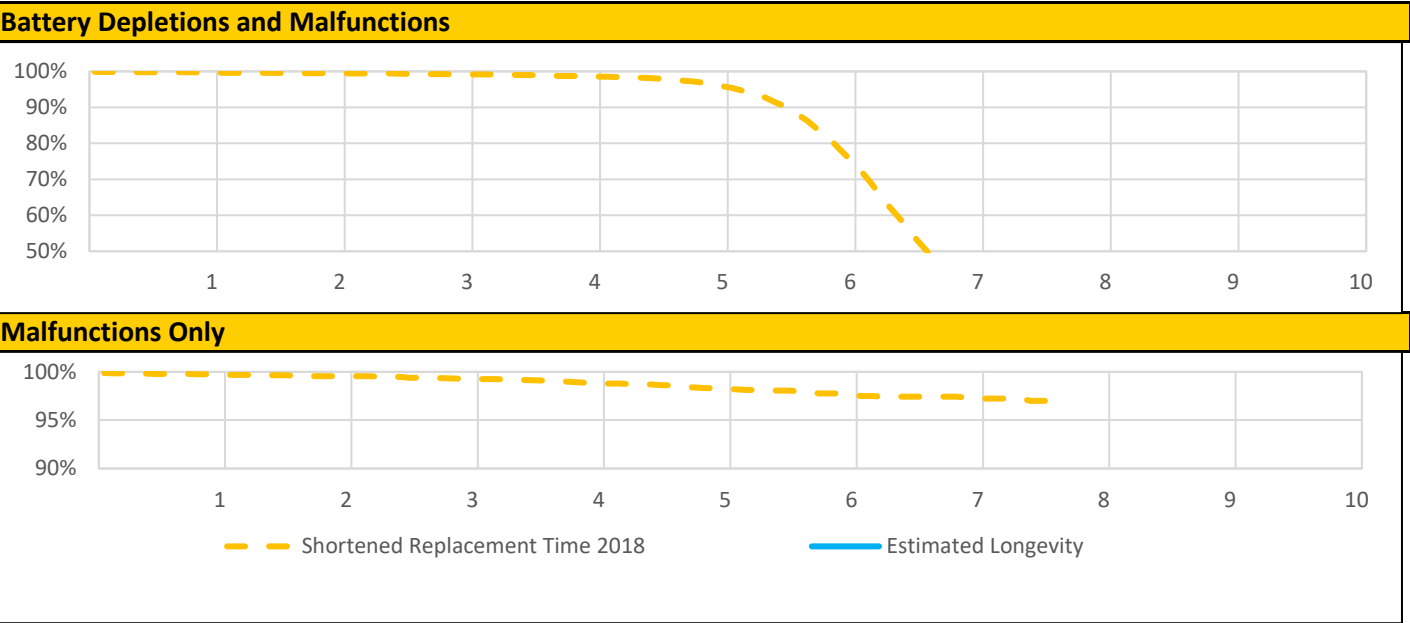

US Survival Probability											
	Year	1	2	3	4	5	6	7	8	9	10
Shortened Replacement Time 2018 Registered Implants:	Depletions and Malfunctions	99.7%	99.5%	99.2%	98.6%	96.4%	78.5%	35.6%	8.8%	--	--
	Malfunctions Only	99.7%	99.5%	99.3%	98.8%	98.3%	97.8%	97.3%	96.6%	--	--
	8,000 Effective Sample Size	6394	5632	4976	4366	3678	2661	1077	231	--	--

@ 93 months

\*Devices subject to an advisory. Refer to the Advisories for more details. Devices may be part of more than one advisory.

# SQ-RX S-ICD

Models: 1010


Worldwide Confirmed Malfunctions		228	
Worldwide Distribution		11,000	
US Approval Date: September 2012	With Compromised Therapy	Without Compromised Therapy	Total
Electrical			
Unintended Fuse Activation 2013 (4)	3	0	3
Charge Timeout Alert (61)	0	11	11
Mechanical			
High cathode condition (5)	1	1	2
Shortened replacement time 2018 (55)	69	46	115
Software			
Unintended Battery Depletion Alert (57)	0	10	10
Other			
Telemetry (56)	10	4	14
Non-patterned, other	42	31	73
Grand Total	125	103	228

References cited in table above [\(link\)](#)

TELIGEN DR

Models: E110/E111/F110/F111

US Summary			
US Registered Implants:	66,000	US Normal Battery Depletions:	12,989
US Approval Date:	March 2008	US Malfunctions:	3,045
US Estimated Active Implants:	14,000	Without Compromised Therapy:	2,878
		With Compromised Therapy:	167

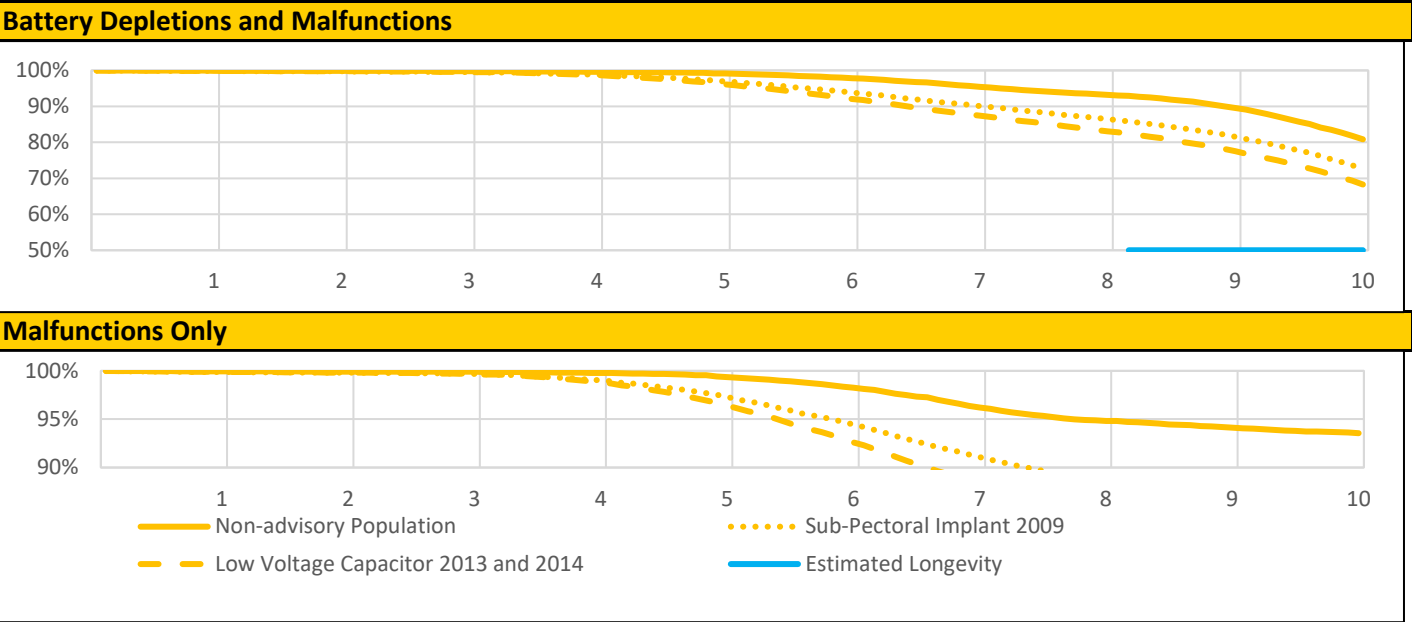

US Survival Probability											
Year		1	2	3	4	5	6	7	8	9	10
Non-Advisory Population	Depletions and Malfunctions	99.9%	99.9%	99.8%	99.6%	99.2%	98.0%	95.7%	93.4%	90.0%	81.8%
Registered Implants:	Malfunctions Only	99.9%	99.9%	99.9%	99.8%	99.4%	98.4%	96.4%	94.9%	94.2%	93.6%
30000	Effective Sample Size	26329	23351	20703	18279	16074	13976	11969	10211	8608	6833

# TELIGEN DR

Models: E110/E111/F110/F111

US Survival Probability (cont.)											
Year		1	2	3	4	5	6	7	8	9	10
Subpectoral Implant 2009	Depletions and Malfunctions	99.9%	99.8%	99.6%	98.9%	97.2%	94.2%	90.4%	86.8%	82.1%	73.7%
	Registered Implants: Malfunctions Only	99.9%	99.8%	99.7%	99.1%	97.5%	94.7%	91.3%	88.6%	86.6%	85.2%
	Effective Sample Size	26621	23498	20766	18232	15836	13489	11345	9481	7784	6029
Low Voltage Capacitor 2013 and 2014	Depletions and Malfunctions	99.9%	99.8%	99.6%	98.8%	96.5%	92.5%	87.8%	83.4%	78.2%	69.3%
	Registered Implants: Malfunctions Only	99.9%	99.8%	99.7%	98.9%	96.7%	93.0%	88.7%	85.3%	82.8%	81.2%
	Effective Sample Size	20609	18214	16087	14112	12158	10237	8506	7031	5705	4357

\*Devices subject to an advisory. Refer to the Advisories for more details. Devices may be part of more than one advisory.

TELIGEN DR


Models: E110/E111/F110/F111

Worldwide Confirmed Malfunctions		4,187	
Worldwide Distribution		91,000	
US Approval Date: March 2008	With Compromised Therapy	Without Compromised Therapy	Total
Electrical			
Low Voltage Capacitor 2014 - August 29, 2013 and September 17, 2014 Voluntary Physician Advisory (3)	54	2299	2353
Safety Core-electrocautery (42)	1	4	5
High-voltage capacitor (43)	8	1	9
Low-voltage capacitors (47)	0	8	8
Integrated circuit (50)	22	22	44
Battery (53)	43	256	299
Low-voltage capacitor (54)	14	1300	1314
Low-voltage capacitor (69)	0	7	7
Mechanical			
Transformer (38)	20	0	20
Seal plug (40)	0	3	3
Difficulty securing lead (41)	8	7	15
Header contacts (45)	12	3	15
Subpectoral implant 2009 - December 01, 2009 Voluntary Physician Advisory (6)	13	9	22
Header (74)	9	3	12
Software			
Alert messages not displayed post-EOL (48)	0	3	3
Memory errors (51)	0	19	19
Other			
Non-patterned, other	11	28	39
Grand Total	215	3972	4187

# TELIGEN VR

Models: E102/E103/F102/F103

US Summary			
US Registered Implants:	38,000	US Normal Battery Depletions:	3,947
US Approval Date:	March 2008	US Malfunctions:	2,419
US Estimated Active Implants:	11,000	Without Compromised Therapy:	2,283
		With Compromised Therapy:	136

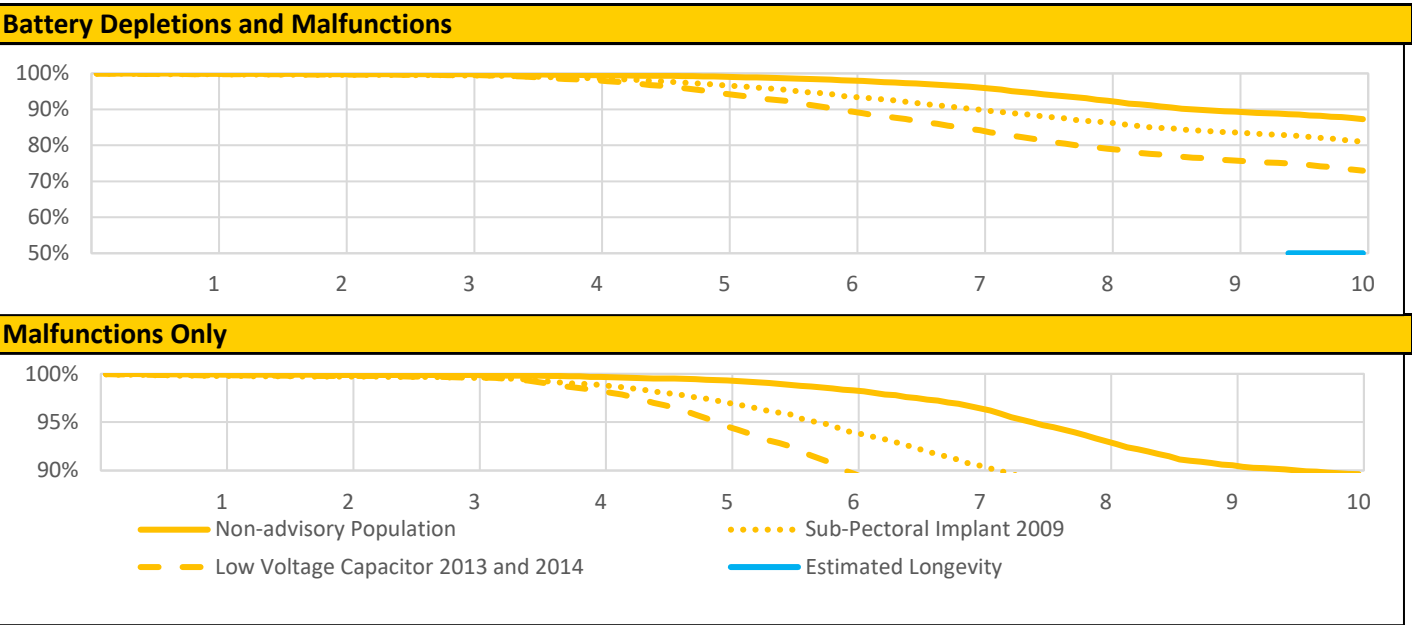

US Survival Probability											
	Year	1	2	3	4	5	6	7	8	9	10
Non-Advisory Population	Depletions and Malfunctions	99.9%	99.8%	99.7%	99.6%	99.1%	98.1%	96.3%	92.7%	89.4%	87.6%
Registered Implants:	Malfunctions Only	99.9%	99.9%	99.9%	99.7%	99.3%	98.4%	96.7%	93.3%	90.6%	89.7%
18000	Effective Sample Size	16093	14234	12564	11073	9714	8447	7241	6048	5069	4354

TELIGEN VR
Models: E102/E103/F102/F103

US Survival Probability (cont.)											
Year		1	2	3	4	5	6	7	8	9	10
Subpectoral Implant 2009	Depletions and Malfunctions	99.8%	99.6%	99.5%	98.7%	96.9%	93.8%	90.1%	86.6%	83.7%	81.3%
	Registered Implants: Malfunctions Only	99.8%	99.7%	99.6%	98.9%	97.2%	94.2%	90.7%	87.4%	84.8%	83.3%
	Effective Sample Size	13605	11987	10561	9233	7977	6788	5696	4742	3981	3344
Low Voltage Capacitor 2013 and 2014	Depletions and Malfunctions	99.8%	99.7%	99.5%	98.2%	94.8%	89.7%	84.6%	79.4%	75.9%	73.3%
	Registered Implants: Malfunctions Only	99.8%	99.8%	99.6%	98.4%	95.0%	90.1%	85.1%	80.2%	77.1%	75.5%
	Effective Sample Size	10845	9573	8438	7355	6256	5187	4238	3434	2846	2375

\*Devices subject to an advisory. Refer to the Advisories for more details. Devices may be part of more than one advisory.

# TELIGEN VR


Models: E102/E103/F102/F103

Worldwide Confirmed Malfunctions		4,104	
Worldwide Distribution		66,000	
US Approval Date: March 2008	With Compromised Therapy	Without Compromised Therapy	Total
Electrical			
Low Voltage Capacitor 2014 - August 29, 2013 and September 17, 2014 Voluntary Physician Advisory (3)	46	1925	1971
Safety Core-electrocautery (42)	1	1	2
High-voltage capacitor (43)	3	0	3
Low-voltage capacitors (47)	0	5	5
Integrated circuit (50)	17	11	28
Battery (53)	55	422	477
Low-voltage capacitor (54)	13	1447	1460
Low-voltage capacitor (69)	0	5	5
Mechanical			
Transformer (24)	1	0	1
Transformer (38)	14	0	14
Seal plug (40)	0	1	1
Difficulty securing lead (41)	9	0	9
Header contacts (45)	22	16	38
Subpectoral implant 2009 - December 01, 2009 Voluntary Physician Advisory (6)	18	12	30
Header (74)	13	4	17
Software			
Alert messages not displayed post-EOL (48)	0	4	4
Memory errors (51)	0	11	11
Respiratory Sensor Oversensing - March 23, 2009 Voluntary Physician Advisory (7)	0	2	2
Other			
Non-patterned, other	13	13	26
Grand Total	225	3879	4104

# ACCOLADE/PROPONENT/ESSENTIO DR

Models: L101/L111/L201/L211/L301/L311

US Summary			
US Registered Implants:	300,000	US Normal Battery Depletions:	9,518
US Approval Date:	April 2016	US Malfunctions:	1,969
US Estimated Active Implants:	237,000	Without Compromised Therapy:	1,876
		With Compromised Therapy:	93

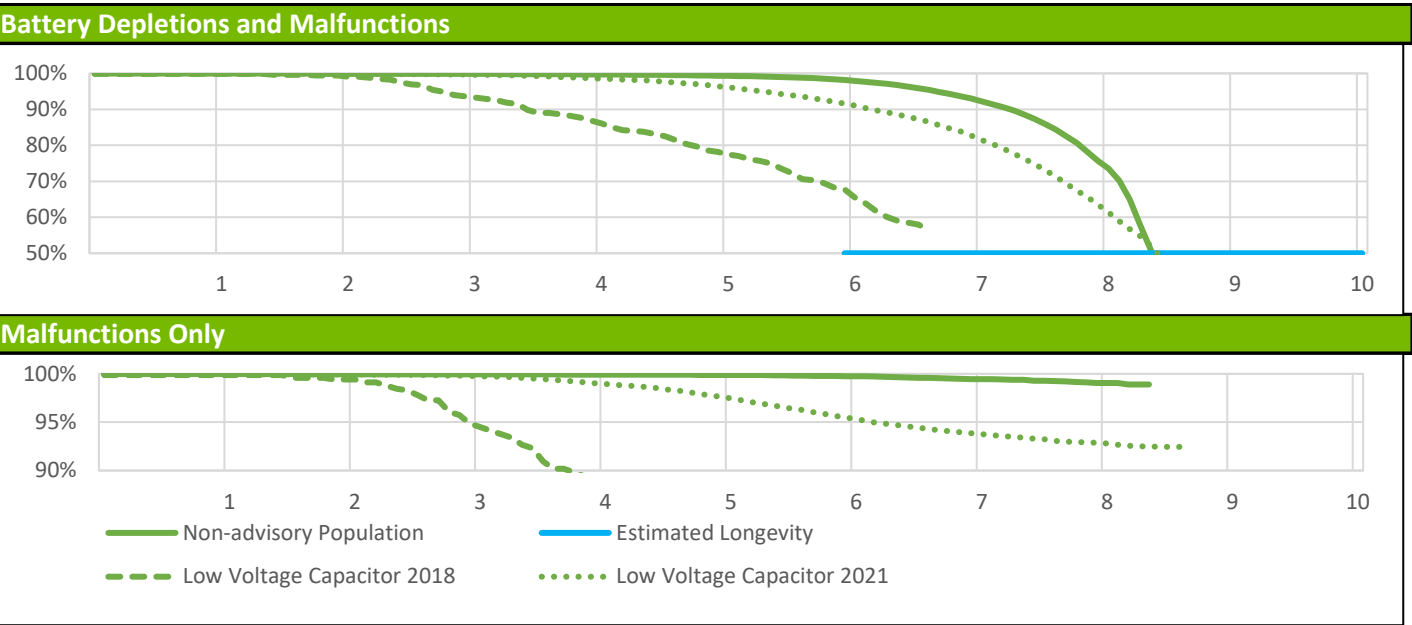

US Survival Probability											
	Year	1	2	3	4	5	6	7	8	9	10
Non-Advisory Population	Depletions and Malfunctions	100.0%	99.9%	99.9%	99.7%	99.4%	98.2%	93.0%	75.7%	43.3%	--
Registered Implants:	Malfunctions Only	100.0%	100.0%	99.9%	99.9%	99.9%	99.8%	99.5%	99.1%	98.9%	--
219000	Effective Sample Size	201973	154755	115470	83395	57440	33942	14690	2673	277	--

@ 102 months

\*Devices subject to an advisory. Refer to the Advisories for more details. Devices may be part of more than one advisory.

# ACCOLADE/PROPONENT/ESSENTIO DR

Models: L101/L111/L201/L211/L301/L311

US Survival Probability (cont.)											
Year		1	2	3	4	5	6	7	8	9	10
Low Voltage Capacitor 2018 Registered Implants: 800	Depletions and Malfunctions	99.9%	99.4%	94.0%	87.7%	78.6%	68.3%	56.2%	--	--	--
	Malfunctions Only	99.9%	99.4%	94.8%	88.8%	83.5%	77.2%	71.8%	--	--	--
	Effective Sample Size	713	640	543	449	361	273	207	--	--	--
Low Voltage Capacitor 2021 Registered Implants: 42000	Depletions and Malfunctions	100.0%	99.9%	99.7%	98.7%	96.4%	91.6%	82.7%	63.4%	32.3%	--
	Malfunctions Only	100.0%	99.9%	99.8%	99.0%	97.6%	95.5%	93.8%	92.9%	92.4%	--
	Effective Sample Size	37245	33198	29497	26065	22695	19102	14273	5635	274	--

@ 81 months

@ 107 months

\*Devices subject to an advisory. Refer to the Advisories for more details. Devices may be part of more than one advisory.

# ACCOLADE/PROPONENT/ESSENTIO DR

Models: L101/L111/L201/L211/L301/L311


Worldwide Confirmed Malfunctions	3,198		
Worldwide Distribution	682,000		
US Approval Date: April 2016	With Compromised Therapy	Without Compromised Therapy	Total
Electrical			
Low-voltage capacitors (47)	2	6	8
Integrated circuit (63)	18	57	75
Capacitor (67)	0	3	3
Telemetry (68)	2	14	16
Hydrogen induced premature depletion - September 2018 (70)	4	222	226
Hydrogen induced premature depletion - June 2021 (83)	48	2185	2233
High battery impedance (89)	18	338	356
Software			
Memory errors (51)	0	74	74
Mechanical			
Battery cathode (79)	6	5	11
Other			
Non-patterned, other	70	126	196
Grand Total	168	3030	3198

References cited in table above [\(link\)](#)

# ACCOLADE/PROPONENT/ESSENTIO EL DR

Models: L121/L131/L221/L231/L321/L331

US Summary			
US Registered Implants:	191,000	US Normal Battery Depletions:	430
US Approval Date:	April 2016	US Malfunctions:	981
US Estimated Active Implants:	167,000	Without Compromised Therapy:	957
		With Compromised Therapy:	24

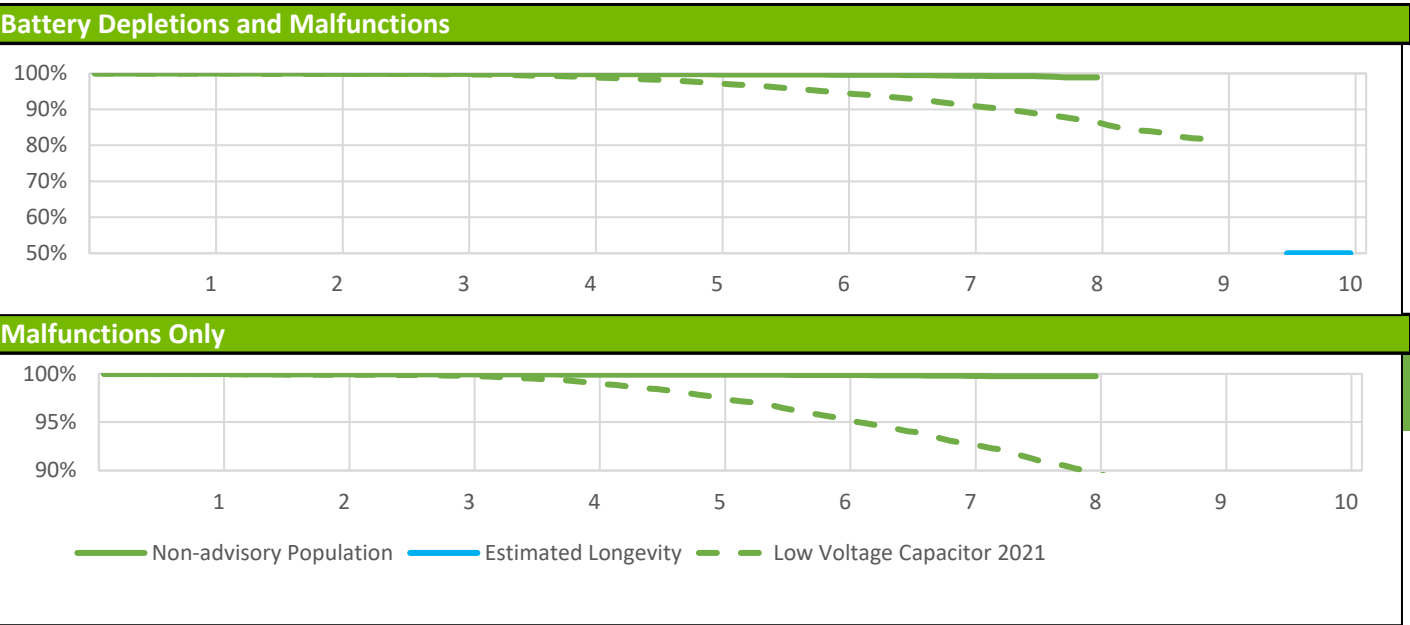

US Survival Probability											
	Year	1	2	3	4	5	6	7	8	9	10
Non-Advisory Population	Depletions and Malfunctions	100.0%	99.9%	99.9%	99.8%	99.7%	99.6%	99.4%	98.9%	98.9%	--
Registered Implants:	Malfunctions Only	100.0%	100.0%	99.9%	99.9%	99.9%	99.9%	99.8%	99.8%	99.8%	--
117,000	Effective Sample Size	128609	92088	63394	41973	26380	14164	5169	456	308	--

@ 97 months

\*Devices subject to an advisory. Refer to the Advisories for more details. Devices may be part of more than one advisory.

# ACCOLADE/PROPONENT/ESSENTIO EL DR

Models: L121/L131/L221/L231/L321/L331

US Survival Probability											
Year		1	2	3	4	5	6	7	8	9	10
Low Voltage Capacitor 2021 Registered Implants: 17,000	Depletions and Malfunctions	100.0%	99.9%	99.7%	98.9%	97.3%	94.6%	91.1%	86.5%	80.8%	--
	Malfunctions Only	100.0%	99.9%	99.8%	99.0%	97.5%	95.2%	92.7%	89.8%	87.9%	--
	Effective Sample Size	14979	13322	11847	10473	9131	7801	6010	2797	229	--

@ 108 months

\*Devices subject to an advisory. Refer to the Advisories for more details. Devices may be part of more than one advisory.

# ACCOLADE/PROPONENT/ESSENTIO EL DR

Models: L121/L131/L221/L231/L321/L331


Worldwide Confirmed Malfunctions		1,994	
Worldwide Distribution		472,000	
US Approval Date: April 2016	With Compromised Therapy	Without Compromised Therapy	Total
Electrical			
Low-voltage capacitors (47)	0	10	10
Integrated circuit (63)	6	48	54
Capacitor (67)	1	1	2
Telemetry (68)	1	14	15
Hydrogen induced premature depletion - September 2018 (70)	3	131	134
Hydrogen induced premature depletion - June 2021 (83)	23	1603	1626
High battery impedance (89)	2	27	29
Software			
Memory errors (51)	0	73	73
Mechanical			
Battery cathode (79)	2	0	2
Other			
Non-patterned, other	10	39	49
Grand Total	48	1946	1994

References cited in table above [\(link\)](#)

# ACCOLADE/PROPONENT/ESSENTIO SR

Models: L100/L110/L200/L210/L300/L310

US Summary			
US Registered Implants:	55,000	US Normal Battery Depletions:	529
US Approval Date:	April 2016	US Malfunctions:	510
US Estimated Active Implants:	39,000	Without Compromised Therapy:	497
		With Compromised Therapy:	13

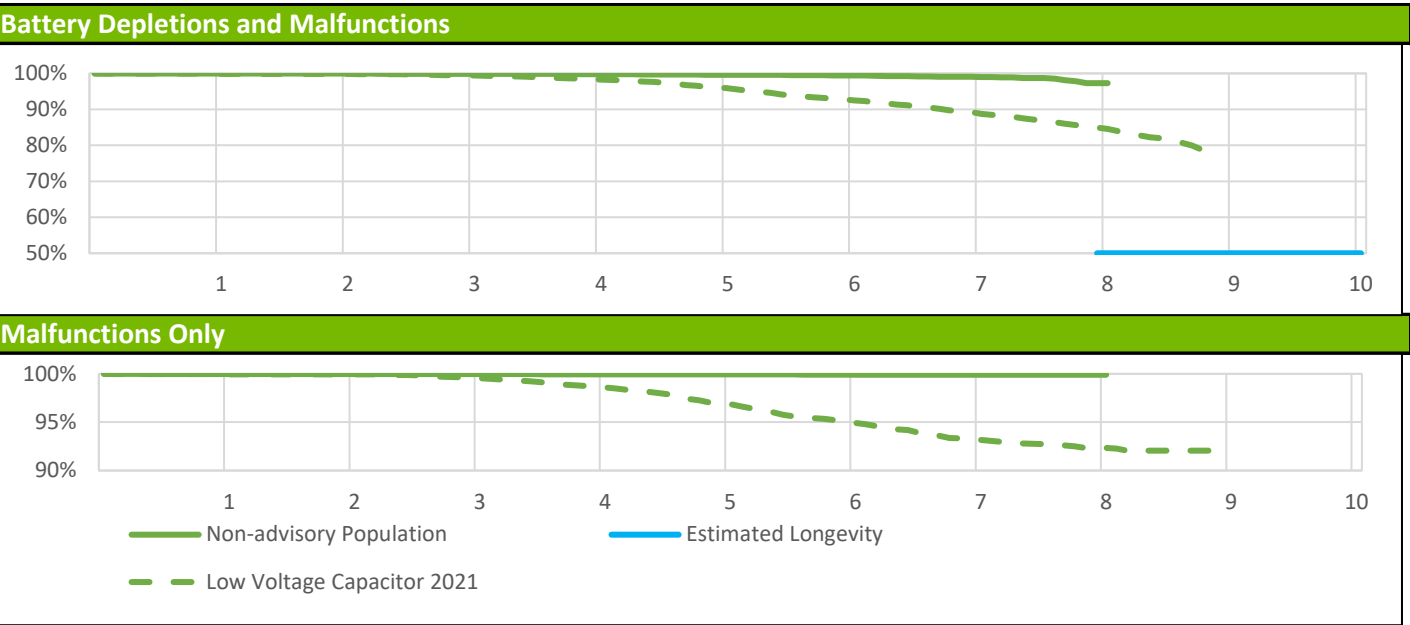

US Survival Probability											
	Year	1	2	3	4	5	6	7	8	9	10
Non-Advisory Population	Depletions and Malfunctions	99.9%	99.9%	99.9%	99.8%	99.6%	99.4%	99.1%	97.3%	97.3%	--
Registered Implants:	Malfunctions Only	100.0%	100.0%	100.0%	100.0%	99.9%	99.9%	99.9%	99.9%	99.9%	--
33,000	Effective Sample Size	32232	25001	18755	13482	9062	5023	1835	285	207	--

@ 97 months

\*Devices subject to an advisory. Refer to the Advisories for more details. Devices may be part of more than one advisory.

# ACCOLADE/PROPONENT/ESSENTIO SR

Models: L100/L110/L200/L210/L300/L310

US Survival Probability											
Year		1	2	3	4	5	6	7	8	9	10
Low Voltage Capacitor 2021 Registered Implants:	Depletions and Malfunctions	99.9%	99.8%	99.4%	98.5%	96.1%	92.8%	89.3%	84.9%	78.4%	--
	Malfunctions Only	100.0%	99.9%	99.6%	98.7%	96.9%	95.1%	93.3%	92.3%	92.1%	--
	12,000 Effective Sample Size	10309	9150	8117	7170	6238	5313	4107	1809	281	--

@ 107 months

\*Devices subject to an advisory. Refer to the Advisories for more details. Devices may be part of more than one advisory.

# ACCOLADE/PROPONENT/ESSENTIO SR

Models: L100/L110/L200/L210/L300/L310

Worldwide Confirmed Malfunctions	1,203
Worldwide Distribution	243,000


US Approval Date: April 2016	With Compromised Therapy	Without Compromised Therapy	Total
Electrical			
Low-voltage capacitors (47)	1	3	4
Integrated circuit (63)	6	7	13
Capacitor (67)	0	3	3
Telemetry (68)	0	4	4
Hydrogen induced premature depletion - September 2018 (70)	3	69	72
Hydrogen induced premature depletion - June 2021 (83)	30	1022	1052
High battery impedance (89)	0	16	16
Software			
Memory errors (51)	0	17	17
Other			
Non-patterned, other	7	15	22
Grand Total	47	1156	1203

References cited in table above [\(link\)](#)

# ADVANTIO/INGENIO/VITALIO/FORMIO DR

Models: J063/J066/J173/J176/J273/J276/J278/J279/K063/K066/K083/K086/K173/K176/K183/K186/K273/K276/K278/K279/  
K283/K286/K288/K289

US Summary			
US Registered Implants:	121,000	US Normal Battery Depletions:	27,609
US Approval Date:	May 2012	US Malfunctions:	320
US Estimated Active Implants:	47,000	Without Compromised Therapy:	300
		With Compromised Therapy:	20

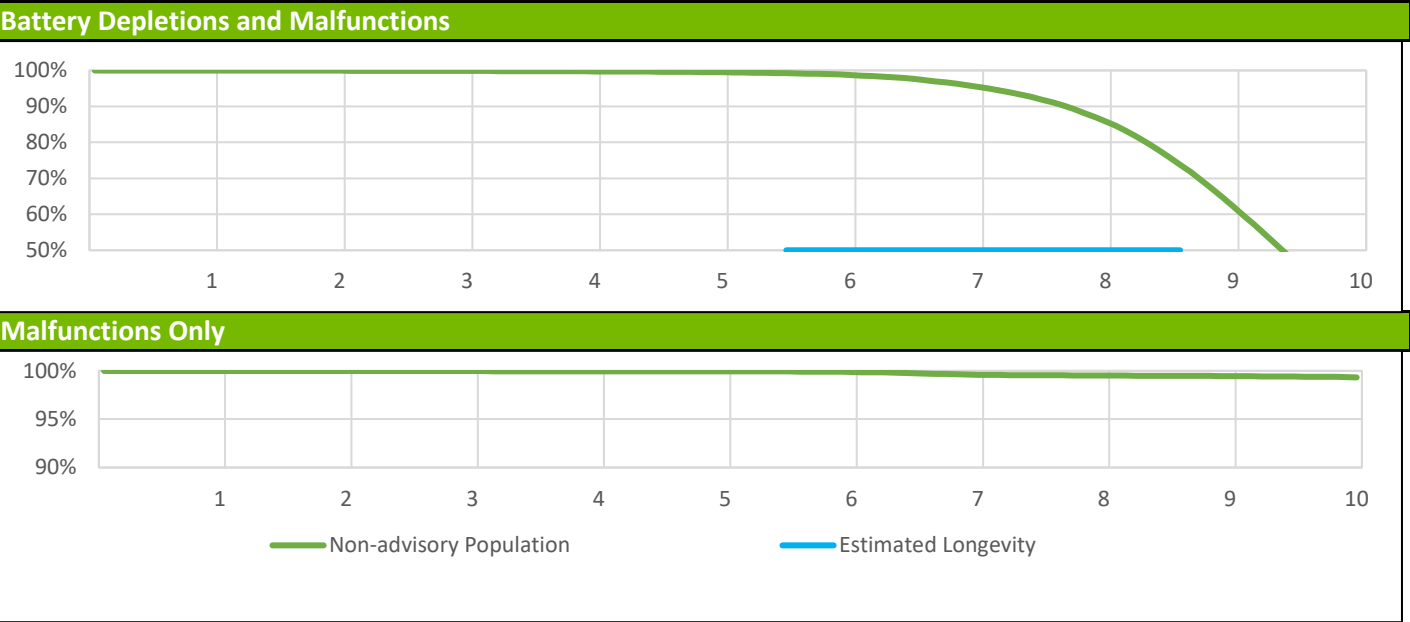

US Survival Probability											
Year		1	2	3	4	5	6	7	8	9	10
Non-Advisory Population	Depletions and Malfunctions	100.0%	99.9%	99.9%	99.7%	99.5%	98.9%	95.9%	87.0%	64.7%	33.8%
Registered Implants:	Malfunctions Only	100.0%	100.0%	100.0%	100.0%	99.9%	99.9%	99.6%	99.5%	99.5%	99.4%
121,000	Effective Sample Size	107310	95719	85349	76074	67632	59917	51814	41898	27098	6609

# ADVANTIO/INGENIO/VITALIO/FORMIO DR

Models: J063/J066/J173/J176/J273/J276/J278/J279/K063/K066/K083/K086/K173/K176/K183/K186/K273/K276/  
K278/K279/K283/K286/K288/K289

Worldwide Confirmed Malfunctions	366
Worldwide Distribution	218,000


US Approval Date: May 2012	With Compromised Therapy	Without Compromised Therapy	Total
Electrical			
Low-voltage capacitors (47)	0	8	8
Integrated circuit (50)	7	3	10
Titanium case material (60)	3	0	3
Software			
Memory errors (51)	1	29	30
Other			
Non-patterned, other	18	297	315
Grand Total	29	337	366

References cited in table above [\(link\)](#)

# ADVANTIO/INGENIO/VITALIO EL DR

Models: J064/J067/J174/J177/J274/J277/K064/K067/K084/K087/K174/K177/K184/K187/K274/K277/K284/K287

US Summary			
US Registered Implants:	11,000	US Normal Battery Depletions:	344
US Approval Date:	May 2012	US Malfunctions:	365
US Estimated Active Implants:	5,000	Without Compromised Therapy:	355
		With Compromised Therapy:	10

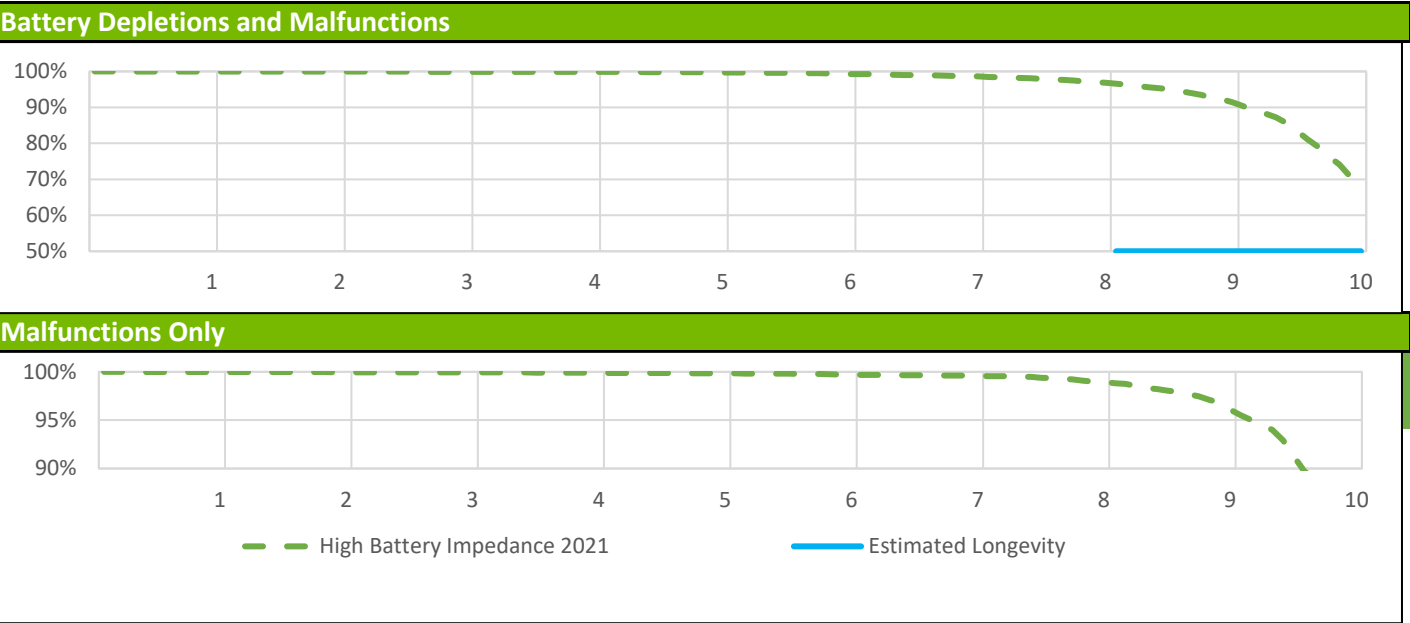

US Survival Probability											
Year		1	2	3	4	5	6	7	8	9	10
High Battery Impedance 2021 Registered Implants: 11,000	Depletions and Malfunctions	100.0%	99.9%	99.9%	99.9%	99.8%	99.3%	98.7%	97.0%	92.2%	70.8%
	Malfunctions Only	100.0%	100.0%	99.9%	99.9%	99.9%	99.7%	99.6%	99.0%	96.8%	81.6%
	Effective Sample Size	9676	8588	7639	6793	6039	5330	4605	3776	2680	501

\*Devices subject to an advisory. Refer to the Advisories for more details. Devices may be part of more than one advisory.

# ADVANTIO/INGENIO/VITALIO/FORMIO EL DR

Models: J064/J067/J174/J177/J274/J277/K064/K067/K084/K087/K174/K177/K184/K187/K274/K277/K284/K287

Worldwide Confirmed Malfunctions	1,020
Worldwide Distribution	75,000


US Approval Date: May 2012	With Compromised Therapy	Without Compromised Therapy	Total
Electrical			
Low-voltage capacitors (47)	1	5	6
Integrated circuit (50)	2	0	2
Titanium case material (60)	2	0	2
High battery impedance initiating safety mode 2021 (82)	27	593	620
Software			
Memory errors (51)	1	11	12
Respiratory sensor (59)	0	1	1
Other			
Non-patterned, other	29	348	377
Grand Total	62	958	1020

References cited in table above [\(link\)](#)

# ADVANTIO/INGENIO/VITALIO/FORMIO SR

Models: J062/J065/J172/J175/J272/J275/K062/K065/K082/K085/K172/K175/K182/K185/K272/K275/K282/K285

US Summary			
US Registered Implants:	27,000	US Normal Battery Depletions:	1,107
US Approval Date:	May 2012	US Malfunctions:	15
US Estimated Active Implants:	12,000	Without Compromised Therapy:	14
		With Compromised Therapy:	1

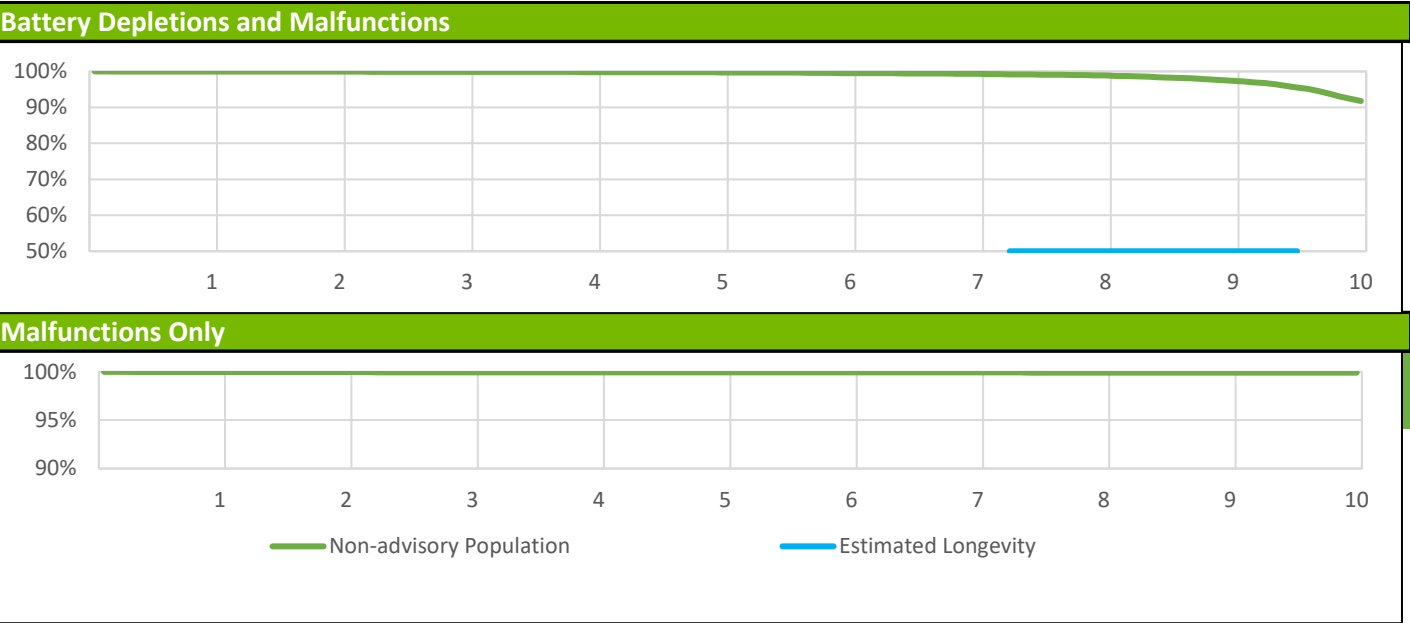

US Survival Probability											
Year		1	2	3	4	5	6	7	8	9	10
Non-Advisory Population	Depletions and Malfunctions	100.0%	99.9%	99.9%	99.8%	99.8%	99.6%	99.4%	98.9%	97.5%	92.4%
Registered Implants:	Malfunctions Only	100.0%	100.0%	100.0%	100.0%	99.9%	99.9%	99.9%	99.9%	99.9%	99.9%
27,000	Effective Sample Size	22795	20265	18071	16129	14377	12808	11428	10123	8311	4484

# ADVANTIO/INGENIO/VITALIO SR

Models: J062/J065/J172/J175/J272/J275/K062/K065/K082/K085/K172/K175/K182/K185/K272/K275/K282/K285

Worldwide Confirmed Malfunctions	30		
Worldwide Distribution	86,000		
US Approval Date: May 2012	With Compromised Therapy	Without Compromised Therapy	Total
Electrical			
Low-voltage capacitors (47)	1	3	4
Integrated circuit (50)	3	2	5
Titanium case material (60)	1	0	1
Software			
Memory errors (51)	0	9	9
Other			
Non-patterned, other	3	8	11
Grand Total	8	22	30

References cited in table above [\(link\)](#)

# ALTRUA 2 DR

Models: S702

Worldwide Confirmed Malfunction:	15
Worldwide Distribution	12,000

CE Mark Date: December 2018	With Compromised Therapy	Without Compromised Therapy	Total
Software			
Memory errors (51)	0	2	2
Electrical			
Hydrogen induced premature depletion - June 2021 (83)	0	11	11
High battery impedance (89)	0	1	1
Integrated circuit (63)	0	1	1
Grand Total	0	15	15

References cited in table above [\(link\)](#)

# ALTRUA 2 EL DR

Models: S722

Worldwide Confirmed Malfunctions	3
Worldwide Distribution	9,000

CE Mark Date: December 2018	With Compromised Therapy	Without Compromised Therapy	Total
Electrical			
Hydrogen induced premature depletion - June 2021 (83)	0	2	2
Other			
Non-patterned, other	0	1	1
Grand Total	0	3	3

References cited in table above [\(link\)](#)

# ALTRUA 2 SR

Models: S701

Worldwide Confirmed Malfunctions		13	
Worldwide Distribution		11,000	
CE Mark Date: December 2018	With Compromised Therapy	Without Compromised Therapy	Total
Electrical			
Hydrogen induced premature depletion - June 2021 (83)	0	11	11
Other			
Non-patterned, other	1	1	2
Grand Total	1	12	13

References cited in table above [\(link\)](#)

## Confirmed Malfunction Details: Pulse Generator References

Descriptions listed below provide an overview of the clinical observations and/or analysis findings associated with each pulse generator confirmed malfunction pattern listed in this report.

All of the patterns listed are thoroughly investigated and analyzed. As part of Boston Scientific's process of continuous improvement, when possible, changes have been or will be implemented in response to identified malfunction patterns. "Improvements implemented" may include product design changes in existing or subsequent generations, manufacturing process modifications, software updates, educational communications, labeling changes, etc. Improvement implementation may vary by geography due to various factors, including regulatory review timing, and may not completely mitigate or eliminate the potential for additional malfunctions.

3. **Low Voltage Capacitor 2014**— *Aug 2013 and Sep 2014 Voluntary Physician Advisory.* Alert message during followup, beeping tones, premature battery depletion. Diminished low voltage capacitor performance. Improvement implemented.
4. **Unintended Fuse Activation 2013**— *March 1, 2013 Voluntary Physician Advisory.* Inability to interrogate, no magnet response, permanent loss of therapy without warning. Improvement implemented.
5. **High cathode condition**— *June 1, 2011 Voluntary Physician Advisory.* Premature battery depletion. Misaligned battery component. Improvement implemented.
6. **Subpectoral implant 2009**— *December 01, 2009 Voluntary Physician Advisory.* Noise, oversensing, inappropriate shocks, pacing inhibition, high impedance when implanted subpectorally. Weakened bond between header and titanium case. Improvement implemented.
7. **Respiratory Sensor Oversensing**— *March 23, 2009 Voluntary Physician Advisory.* Oversensing, noise, inappropriate shock, pacing inhibition. When Respiratory Sensor is ON, RV lead or system complications may cause oversensing or noise. Improvement implemented.
8. **Low-voltage capacitor**— *June 23, 2006 and August 24, 2006 Voluntary Physician Advisory.* Premature battery depletion, no output, no interrogation. Failed low-voltage capacitor. Improvement implemented.
9. **Crystal timing component Failure Mode 1**— *September 22, 2005 Voluntary Physician Advisory.* Intermittent or permanent loss of pacing output without warning, intermittent or permanent loss of telemetry, reversion to VVI mode or appearance of a reset warning message upon interrogation. Foreign material within a crystal timing component. Improvement implemented.
10. **Crystal timing component Failure Mode 2**— *September 22, 2005 Voluntary Physician Advisory.* At implant procedure or during pre-implant testing: Intermittent or permanent loss of pacing output without warning, intermittent or permanent loss of telemetry, reversion to VVI mode, or appearance of a reset warning message upon interrogation. Microscopic particle within a crystal timing component. Three failures have been reported following confirmation of successful implantation. No currently distributed devices are subject to this peri-implant failure mode. Improvement implemented.
11. **Longevity labeling**— Battery longevity inconsistent with longevity labeling. Device battery status indicators are accurate and no loss of therapy has been reported.
12. **Solder bond**— Loss of device output, loss of sensing. Separation of component solder from substrate. Improvement implemented.
13. **Integrated circuit**— Power on Reset state, loss of telemetry, safety mode operation or loss of output. Failed digital integrated circuit.
14. **Capacitor**— Premature battery depletion, inability to interrogate. Damage to low-voltage capacitor.
15. **Capacitor**— No telemetry, no pacing, premature battery depletion. Gradual, premature battery depletion most common; in rare instances, rapid depletion occurred with no therapy available. Failed low-voltage capacitor.
16. **Capacitor array**— Loss of device output, loss of capture, inability to accurately measure charge times causing elective replacement indicator declaration. Damage to capacitor array. Improvement implemented.
17. **Integrated circuit**— No telemetry, premature battery depletion. Integrated circuit issue within high-voltage transistor.
18. **Battery depletion**— Premature battery depletion and loss of capture.
19. **Seal plug**— Non-cardiac signals on electrograms leading to inhibition of pacing and/or inappropriate shock delivery. Damaged seal plug. Improvement implemented.
20. **Header**— High impedance, compromised header bonding identified during lead revision procedures. Insufficient medical adhesive bonding between header and case. Improvement implemented.
21. **Magnet response**— No magnet response. Particulate material in component. Improvement implemented.
22. **Battery depletion**— Premature battery depletion.
23. **Memory error**— Device resets (including pacing at reset parameters) and inability to interrogate. Errors in device memory.
24. **Transformer**— Charge time alert message and/or end of life (EOL) indicator displayed, loss of shock therapy. Damaged transformer. Improvement implemented.
25. **Setscrew block**— No pacing or pauses in pacing, intermittent or lack of setscrew contact with lead. Incorrect setscrew block. Improvement implemented.
26. **Battery depletion**— Loss of therapy, inability to interrogate, no magnet response, premature battery depletion.

27. **Solder bond**— Inability to interrogate, no magnet response, no pacing output. Broken solder bond between wire mounting surface and internal circuitry. Improvement implemented.
28. **Stored EGMs**— Inability to view stored EGMs. Incorrect EGM index location.
29. **Battery post**— Inability to interrogate, no pacing output. Bent battery post. Improvement implemented.
30. **Integrated circuit**— Premature battery depletion, loss of pacing output, inability to interrogate, loss of sensing, high-rate pacing, loss of shock therapy. Damage to integrated circuit. Improvement implemented.
31. **Alert messages**— During programmer interactions, alert messages appear which are able to be cleared. In one case, an alert message occurred with two memory errors after multiple device resets.
32. **Setscrew**— Inability to tighten or loosen setscrews during implant or replacement procedure due to process variability. Improvement implemented.
33. **Seal plug**— Lifted or missing seal plugs. Inadequate medical adhesive bond. Improvement implemented
34. **Underestimation of battery status**— Underestimation of remaining longevity due to invalid charge time measurement. Improvement implemented.
35. **Interrupted telemetry**— Early appearance of Elective Replacement Time (ERT) indicator, unexpected impedance measurements (>2500 ohms). Interruption in telemetry sequence during software upgrade. Improvement implemented.
36. **Pacing rate limit**— Inability to interrogate. Inappropriate pacing due to feature interaction. Improvement implemented.
37. **Solder joint**— Inappropriate shocks, beeping, fallback mode, errors or inability to interrogate or program. Cracked solder joint due to repetitive mechanical stress-induced component damage, only when implanted subpectorally with serial number facing the ribs.
38. **Transformer**— Inability to interrogate, loss of pacing and shock therapy. Failed transformer.
39. **Connector block**— Connector block can be moved out of alignment or displaced from header. Prolonged implant procedure, high impedance, no pacing, no sensing. Improvement implemented.
40. **Seal plug**— Non-cardiac signals on electrograms may result in loss of pacing or inappropriate shocks. Seal plug allows air in lead port to escape.
41. **Difficulty securing lead**— Noise, high impedance, inappropriate shocks or loss of therapy due to crossthreaded setscrews, intermittent or lack of contact between lead and header. Improvement implemented.
42. **Safety Core-electrocautery**— During electrocautery, device may enter Safety Core. Circuitry response to noise caused by electrocautery. Improvement implemented.
43. **High-voltage capacitor**— Alert message upon interrogation, extended charge time. Damaged high voltage capacitor.
44. **Magnet rate**— During interrogation, magnet rate remains after removal of magnet. Reed switch stuck in closed position. Improvement implemented.
45. **Header contacts**— Noise, oversensing, inappropriate shock, high pacing impedance, possible loss of pacing and sensing. Poor header connection with lead terminals due to contacts.
46. **Safety Core-programming**— Device enters Safety Core after three consecutive invalid programming attempts, due to firmware issue. Improvement implemented.
47. **Low-voltage capacitors**— Premature battery depletion, voltage alert during followup, device beeping. Capacitor failure.
48. **Alert messages not displayed post-EOL**— No alert message display after EOL declaration. Improvement implemented.
49. **Battery status**— Longevity remaining, battery status, gas gauge and/or magnet rate do not align or are inconsistent.
50. **Integrated circuit**— Loss of telemetry, premature battery depletion, alert message during followup. Integrated circuit issue. Improvement implemented.
51. **Memory errors**— Safety mode operation, inaccurately labeled pacing data. Errors in device memory
52. **High voltage circuit**— Alert message after implant, loss of shock therapy. Failed output module.
53. **Battery**— Beeping tones and alert message upon interrogation. Reduced battery voltage. Improvement implemented.
54. **Low-voltage capacitor**— Alert message during followup, beeping tones, premature battery depletion. Diminished low voltage capacitor performance. Improvement implemented.
55. **Shortened replacement time 2018 November 2018 Voluntary Physician Advisory**. Premature, gradual depletion of battery; in rare instances, rapid depletion with no therapy available. Improvement implemented.
56. **Telemetry**— Inability to interrogate, premature battery depletion.
57. **Unintended Battery Depletion Alert**— Beeping tones, Battery Depletion alert during followup despite normal battery depletion. Alert may be cleared without impact to battery status or therapy availability. Improvement implemented.
58. **High voltage circuit**— Long charge time at implant, inability to interrogate, loss of pacing and shock therapy. Improvement implemented.
59. **Respiratory sensor**— Temporary increase or decrease in pacing rate as a result of respiratory sensor response to non-respiratory signals. No loss of pacing output.
60. **Titanium case material**— Noise, oversensing, abnormal pacing impedance, loss of capture, premature battery depletion. Titanium case material creating a higher than normal current drain condition. Improvement implemented.
61. **Charge Timeout Alert**— Beeping tones, programmer warning screen, abnormal shock impedance. Charge timeout alert.
62. **High voltage circuit component**— Charge time alert message and/or Elective Replacement indicator (ERI) displayed, beeping tones. High voltage circuit component. Improvement implemented.
63. **Integrated circuit**— Abnormal lead impedance, no telemetry, premature battery depletion. Integrated circuit issue within high-voltage transistor Improvement implemented

64. **Safety Core-unintended biventricular pacing**— *Dec 2017 Voluntary Physician Advisory*. Device enters Safety Core after detecting unintended asynchronous biventricular pacing due to software issue.
65. **Memory corruption** - *Jun 2017 Voluntary Physician Advisory*. Atypical energy delivery, error messages upon interrogation, loss of tachy therapy. Memory corruption. Improvement implemented.
67. **Capacitor**— Premature battery depletion. Diminished low voltage capacitor performance.
68. **Telemetry**— Alert message during followup, inability to interrogate, premature battery depletion, loss of pacing therapy. Telemetry component.
69. **Low-voltage capacitor**— Alert message during followup, beeping tones, premature battery depletion.
70. **Hydrogen induced premature depletion - September 2018 - September 2018 Voluntary Physician Advisory**. Premature battery depletion. Diminished low voltage capacitor performance.
71. **Battery** – Premature, gradual depletion of battery; in rare instances, rapid depletion with no therapy available. Improvement implemented.
72. **Capacitor**— Premature battery depletion. Diminished capacitor performance
73. **Misaligned markers**— Stored episode markers do not match recorded EGM.
74. **Header**— Noise, oversensing, inappropriate shocks, pacing inhibition, high impedance when implanted subcutaneously. Weakened bond between header and titanium case. Improvement Implemented.
75. **High voltage capacitor**— Charge time alert message, end of life (EOL) indicator displayed, beeping tones. Loss of tachy therapy without loss of brady therapy. Internal high-voltage capacitor issue. Improvement implemented.
76. **Internal insulation**— Beeping tones, loss of telemetry, premature battery depletion, loss of tachy therapy. Internal insulation issue.
77. **S-ICD battery depletion 2019 and 2020 – August 2019 and December 2020 Voluntary Physician Advisory**. Premature battery depletion. Diminished capacitor performance.
78. **Solder joint**— Beeping tones, device errors, loss of tachy therapy. Cracked solder joint.
79. **Battery cathode**— Safety mode operation, inability to interrogate, loss of brady therapy. Internal battery cathode issue.
80. **EMBLEM S-ICD electrical overstress 2020— December 2020 Voluntary Physician Advisory**. Beeping tones, loss of telemetry, loss of sensing, premature battery depletion, loss of tachy therapy.
81. **RF antenna**— Beeping tones, loss of telemetry, loss of sensing, premature battery depletion, loss of tachy therapy. Exposed antenna issue.
82. **High battery impedance initiating safety mode 2021— June 2021 Voluntary Physician Advisory**. Safety mode operation, system resets. Temporary reduction in battery voltage later in device life.
83. **Hydrogen induced premature depletion June 2021— June 2021 Voluntary Physician Advisory**. Premature battery depletion. Diminished low voltage capacitor performance.
84. **Battery depletion**— Beeping tones, device errors, premature battery depletion.
85. **Memory corruption**— Inability to interrogate, error messages upon interrogation, inappropriate shocks, loss of tachy therapy, and/or inaccurate patient information. Product returned with evidence of transient memory corruption.
86. **Cracked case**— Error messages upon interrogation, inability to interrogate, inappropriate shocks, loss of tachy therapy. Cracked outer case.
87. **Header**— Inability to interrogate, loss of tachy therapy. Header insulation issue.
88. **Solder joint**— Error messages upon interrogation, low impedance measurements, loss of tachy therapy. Fractured solder joint.
89. **High battery impedance**— Safety mode operation, system resets. Battery performance not as intended.

# Before/During Implant Procedure - Worldwide Malfunctions: Pulse Generators

This section of the report depicts the number of product malfunctions that occurred worldwide either before implant (prior to opening the sterile product packaging) or during implant (once the sterile product packaging has been opened). In all cases, the product in question must be returned to Boston Scientific CRM and confirmed through laboratory analysis to have operated or exhibited a problem outside the specified performance limits established by Boston Scientific. Damage incurred during shipping/transit or due to external factors warned against in labeling (e.g. radiation) is not reported as device malfunction here.

The Electrical category is comprised of confirmed malfunctions involving electrical components such as batteries and capacitors, and also includes fault codes encountered at implant. The majority of before/during implant pulse generator confirmed malfunctions in the Mechanical category are issues occurring within the connector block (e.g. stuck setscrews, seal plug/ring issues). The Software category consists primarily of confirmed malfunctions that result in telemetry issues. Confirmed malfunctions in the Labeling and Packaging categories include product labeling/identification issues and damage to sterile packaging, respectively. The Other category is comprised of non-patterned confirmed malfunctions.

CRT-D/Model	Worldwide Distribution	Electrical	Mechanical	Software	Other	Labeling	Packaging
RESONATE/MOMENTUM/CHARISMA/VIGILANT CRT-D G124/G125/G126/G128/G138/G224/G225/G228/G237/G247/ G248/G324/G325/G347/G348/G424/G425/G426/G428/G437/ G447/G448/G524/G525/G526/G528/G537/G547/G548	164,000	2	2	7	15	0	0
AUTOGEN CRT-D G160/G161/G164/G166/G168/G172/G173/G175/ G177/G179	25,000	3	0	0	4	0	0
DYNAGEN/INOGEN/ORIGEN CRT-D G150/G151/G154/G156/G158/G140/G141/ G146/G148/G050/G051/G056/G058	136,000	3	4	5	17	0	0
CRT-P/Model	Worldwide Distribution	Electrical	Mechanical	Software	Other	Labeling	Packaging
VISIONIST/VALITUDE U125/U128//U225/U226/U228	120,000	5	0	2	7	0	0
INTUA/INVIVE/INLIVEN V272/V273/V282/V283/W272/W273/V172/V173/V182/V183/W172/ W173	24,000	0	0	1	6	0	0

ICD/Model	Worldwide Distribution	Electrical	Mechanical	Software	Other	Labeling	Packaging
<b>RESONATE/MOMENTUM/CHARISMA/VIGILANT ICD DR</b> D121/D221/D233/D321/D333/D421/D433/D521/D533	106,000	1	2	8	8	0	0
<b>RESONATE/MOMENTUM/CHARISMA/VIGILANT ICD VR</b> D120/D220/D232/D320/D332/D420/D432/D520/D532	77,000	1	5	2	4	0	0
<b>PERCIVA ICD DR</b> D160/D161/D174/D175	10,000	0	0	0	0	0	0
<b>PERCIVA ICD VR</b> D160/D161/D174/D175	7,000	0	0	1	0	0	0
<b>AUTOGEN ICD EL VR</b> D160/D161/D174/D175	17,000	1	0	0	0	0	0
<b>AUTOGEN ICD EL DR</b> D162/D163/D176/D177	16,000	1	0	1	0	0	0
<b>DYNAGEN/INOGEN/ORIGEN ICD EL VR</b> D020/D021/D010/D011/D000/D001	76,000	1	0	3	4	0	0
<b>DYNAGEN/INOGEN/ORIGEN ICD EL DR</b> D020/D021/D010/D011/D000/D001	86,000	0	3	2	3	0	0
<b>DYNAGEN/INOGEN/ORIGEN ICD MINI VR</b> D020/D021/D010/D011/D000/D001	35,000	1	0	4	2	0	0
<b>DYNAGEN/INOGEN/ORIGEN ICD MINI DR</b> D022/D023/D012/D013/D002/D003	34,000	2	0	0	3	0	0
S-ICD/Model	Worldwide Distribution	Electrical	Mechanical	Software	Other	Labeling	Packaging
<b>EMBLEM S-ICD</b> A209/A219	148,000	2	0	5	133	0	0
<b>SQ-RX S-ICD</b> 1010	11,000	11	0	21	27	0	0

Pacemaker/Model	Worldwide Distribution	Electrical	Mechanical	Software	Other	Labeling	Packaging
ACCOLADE/PROPONENT/ESSENTIO DR EL J064/K064/K067/K084	472,000	8	3	12	19	0	0
ACCOLADE/PROPONENT/ESSENTIO DR J064/K064/K067/K084	682,000	6	0	14	32	0	0
ACCOLADE/PROPONENT/ESSENTIO SR L100/L110/L200/L210/L300/L310	243,000	4	1	7	18	0	0
ADVANTIO/INGENIO/VITALIO EL DR J064/J067/K064/K067/K084/K087/ J174/J177/K174/K177/K184/K187/ J274/J277/K274/K277/K284/K287	75,000	1	1	0	4	0	0
ADVANTIO/INGENIO/VITALIO/FORMIO DR J064/J067/K064/K067/K084/K087/J174/J177/ K174/K177/K184/K187/J274/J277/K274/K277/ K284/K287/J278/J279/K278/K279/K288/K289	218,000	4	0	1	15	0	0
ADVANTIO/INGENIO/VITALIO SR J062/J065/K062/K065/K082/K085/ J172/J175/K172/K175/K182/K185/ J272/J275/K272/K275/K282/K285	86,000	0	0	1	5	0	0

## U.S. Reason for Out of Service

As requested by the Heart Rhythm Society Task Force on Device Performance Policies and Guidelines, Boston Scientific provides reasons for device explant or out of service, if known. The reasons consist of normal battery depletion, unconfirmed premature battery depletion, device upgrade, device malfunction (which includes devices under advisory that have experienced a malfunction), complication related to another system component or clinical condition, (such as infection), or "other," a category consisting of patient death, prophylactic device explant, elective replacement, general product dissatisfaction, other observation/complication, unspecified, or unknown.

The counts for normal battery depletion, unconfirmed premature battery depletion, and device malfunction are reflected in the U.S. survival probability data. Reason for device explant or out of service may either be confirmed through laboratory analysis (as in the case of device malfunction) or it may be reported to Boston Scientific with no associated device return or laboratory analysis. Although a device may be indicated by the health care provider to have been taken out of service for more than one reason, the table below indicates only one reason per device in category counts.

CRT-D/Model	U.S. Registered Implants	Normal Battery Depletion	Device Upgrade	Device Malfunction <sup>1</sup>	Complication related to another system component or clinical condition <sup>2</sup>	Other <sup>3</sup>
<b>RESONATE/MOMENTUM/CHARISMA/VIGILANT CRT-D</b> G124/G125/G126/G128/G138/G224/G225/G228/G237/G247/G248/G324/G325/G347/G348/G424/G425/G426/G428/G437/G447/G448/G524/G525/G526/G528/G537/G547/G548	89000	254	401	50	1131	6978
<b>DYNAGEN/INOGEN/ORIGEN CRT-D</b> G050/G051/G056/G058/G140/G141/G146/G148/G150/G151/G154/G156/G158	76000	3074	555	131	1346	15127
<b>INCEPTA/ENERGEN/PUNCTUA CRT-D</b> N050/N051/N052/N053/N140/N141/N142/N143/N160/N161/N162/N163/N164/N165/P052/P053/P142/P143/P162/P163/P165	53000	11490	516	821	960	20321
<b>COGNIS</b> N118/N119/N120/P106/P107/P108	75000	15945	445	2111	1693	40254
CRT-P/Model	U.S. Registered Implants	Normal Battery Depletion	Device Upgrade	Device Malfunction <sup>1</sup>	Complication related to another system component or clinical condition <sup>2</sup>	Other <sup>3</sup>
<b>VISIONIST/VALITUDE</b> U125/U128/U225/U226/U228	58000	877	1364	208	459	8463
<b>INTUA/INVIVE/INLIVEN</b> V272/V273/V282/V283/W272/W273/V172/V173/V182/V183/W172/W173	10000	1246	228	590	79	5006
<b>CONTAK RENEWAL TR</b> H120/H125	19000	4327	218	67	211	12073

<b>S-ICD/Model</b>	U.S. Registered Implants	Normal Battery Depletion	Device Upgrade	Device Malfunction <sup>1</sup>	Complication related to another system component or clinical condition <sup>2</sup>	Other <sup>3</sup>
EMBLEM S-ICD A209, A219	64000	1421	901	4874	1276	6744
SQ-RX S-ICD 1010	8000	2985	231	117	252	1987

<b>ICD/Model</b>	U.S. Registered Implants	Normal Battery Depletion	Device Upgrade	Device Malfunction <sup>1</sup>	Complication related to another system component or clinical condition <sup>2</sup>	Other <sup>3</sup>
RESONATE/MOMENTUM/CHARISMA/VIGILANT ICD DR D121/D221/D233/D321/D333/D421/D433/D521/D533	58000	39	1403	23	592	2894
RESONATE/MOMENTUM/CHARISMA/VIGILANT ICD VR D120/D220/D232/D320/D332/D420/D432/D520/D532	32000	16	909	18	334	1499
DYNAGEN/INOGEN/ORIGEN ICD EL DR D052/D053/D142/D143/D152/D153	50000	119	2687	114	747	6871
DYNAGEN/INOGEN/ORIGEN ICD EL VR D050/D051/D140/D141/D150/D151	39000	59	2428	103	573	5071
DYNAGEN/INOGEN/ORIGEN ICD MINI DR D002/D003/D012/D013/D022/D023	11000	2395	510	23	149	2210
DYNAGEN/INOGEN/ORIGEN ICD MINI VR D000/D001/D010/D011/D020/D021	10000	1534	539	18	146	1791
INCEPTA/ENERGEN/PUNCTUA ICD VR E050/E051/E140/E141/E160/E160/ F050/F051/F140/F141/F160/F161	39000	629	2783	1328	594	11188
INCEPTA/ENERGEN/PUNCTUA ICD DR E052/E053/E142/E143/E162/E163/F052/F053/F142/F143/F162/F163	47000	2980	3119	1299	738	14477

ICD/Model, continued...	U.S. Registered Implants	Normal Battery Depletion	Device Upgrade	Device Malfunction <sup>1</sup>	Complication related to another system component or clinical condition <sup>2</sup>	Other <sup>3</sup>
TELIGEN VR E102/E103/F102/F103	38000	3940	2173	2427	686	17379
TELIGEN DR E110/E111/F110/F111	66000	12983	3069	3056	1166	31598

Pacemaker/Model	U.S. Registered Implants	Normal Battery Depletion	Device Upgrade	Device Malfunction <sup>1</sup>	Complication related to another system component or clinical condition <sup>2</sup>	Other <sup>3</sup>
ACCOLADE/PROPONENT/ESSENTIO DR EL L121/L131/L221/L231/L321/L331	190000	429	5731	981	1028	15002
ACCOLADE/PROPONENT/ESSENTIO DR L101/L111/L201/L211/L301/L311	299000	9483	8333	1979	1566	41135
ACCOLADE/PROPONENT/ESSENTIO SR L100/L110/L200/L210/L300/L310	55000	527	2003	511	269	12002
ADVANTIO/INGENIO/VITALIO EL DR J064/J067/K064/K067/K084/K087/ J174/J177/K174/K177/K184/K187/ J274/J277/K274/K277/K284/K287	11000	344	531	365	61	4359
ADVANTIO/INGENIO/VITALIO/FORMIO DR J064/J067/K064/K067/K084/K087/J174/J177/ K174/K177/K184/K187/J274/J277/K274/K277/ K284/K287/J278/J279/K278/K279/K288/K289	121000	27579	4256	322	583	41162
ADVANTIO/INGENIO/VITALIO SR J062/J065/K062/K065/K082/K085/ J172/J175/K172/K175/K182/K185/ J272/J275/K272/K275/K282/K285	27000	1106	773	16	114	12293

<b>Pacemaker/Model, continued...</b>	U.S. Registered Implants	Normal Battery Depletion	Device Upgrade	Device Malfunction <sup>1</sup>	Complication related to another system component or clinical condition <sup>2</sup>	Other <sup>3</sup>
ALTRUA 60 SR S601	32000	3901	498	31	146	18856
ALTRUA 60 DR (Downsize) S603	90000	26130	1263	103	464	41471
ALTRUA 60 DR S602	22000	4933	506	46	165	10503
ALTRUA 60 DR EL S606	59000	11079	1549	94	359	25467
ALTRUA 40 SR S401	5000	542	55	2	17	3056
ALTRUA 40 DR (downsize) S403	14000	4074	167	5	65	6960
ALTRUA 40 DR S402	2000	323	33	2	6	980
ALTRUA 40 DR EL S404	5000	825	93	8	34	2631
ALTRUA 20 SR S201/S204	5000	297	46	3	31	3040
ALTRUA 20 DR EL S208	3000	323	53	6	10	1732

<sup>1</sup> Device malfunction consists of all U.S. confirmed malfunctions for a product/product grouping. These include confirmed malfunctions for advisory populations, as well as any other type of malfunction in which a device was returned and confirmed by laboratory analysis to have malfunctioned.. U.S. confirmed malfunction counts are reflected in U.S. survival probability.


<sup>2</sup> System component and/or clinical condition complications may include, for example: infection, erosion, lead-to-PG interface.

<sup>3</sup> Other consists of: patient death, elective replacement, general product dissatisfaction, other observation/complication, unspecified, or unknown.

# ACUITY X4 Spiral L

Models: 4677/4678

US Summary			
US Registered Implants:	22,000	US Chronic Complications	57
US Approval Date:	February 2016	US Malfunctions:	1
US Estimated Active Implants:	19,000	Without Compromised Therapy:	1
		With Compromised Therapy:	-

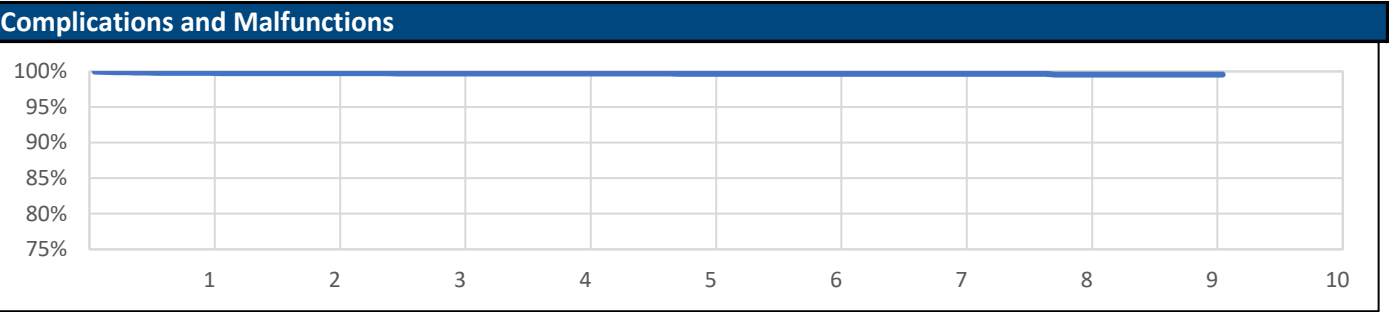

US Survival Probability											
Year		1	2	3	4	5	6	7	8	9	10
Non-Advisory Population	Complications and Malfunctions	99.8%	99.7%	99.7%	99.7%	99.7%	99.7%	99.7%	99.6%	99.6%	99.6%
Registered Implants: 22000	Effective Sample Size	17683	14017	10892	8223	5956	3764	1970	658	227	211

@ 109 months

# ACUITY X4 Spiral L

Models: 4677/4678


Worldwide Confirmed Malfunctions		2	
Worldwide Distribution		54,000	
US Approval Date: February 2016			
	With Compromised Therapy	Without Compromised Therapy	Total
Other			
Non-patterned, other	0	2	2
Grand Total	0	2	2

References cited in table above [\(link\)](#)

# ACUITY X4 Spiral S

Models: 4674/4675

US Summary			
US Registered Implants:	67,000	US Chronic Complications	153
US Approval Date:	February 2016	US Malfunctions:	1
US Estimated Active Implants:	58,000	Without Compromised Therapy:	1
		With Compromised Therapy:	-

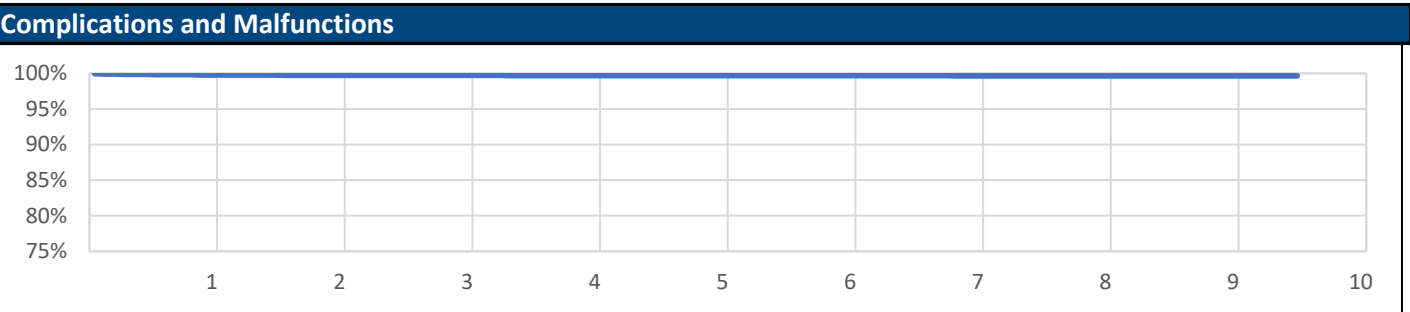

US Survival Probability											
Year		1	2	3	4	5	6	7	8	9	10
Non-Advisory Population	Complications and Malfunctions	99.8%	99.8%	99.7%	99.7%	99.7%	99.7%	99.7%	99.7%	99.7%	99.7%
Registered Implants: 67000	Effective Sample Size	52571	40868	30947	22640	15576	9541	4886	1303	336	224

@ 114 months

# ACUITY X4 Spiral S

Models: 4674/4675


Worldwide Confirmed Malfunctions		1	
Worldwide Distribution		143,000	
US Approval Date: February 2016			
	With Compromised Therapy	Without Compromised Therapy	Total
Other			
Non-patterned, other	0	1	1
Grand Total	0	1	1

References cited in table above [\(link\)](#)

# ACUITY X4 Straight

Models: 4671/4672

US Summary			
US Registered Implants:	50,000	US Chronic Complications	280
US Approval Date:	February 2016	US Malfunctions:	2
US Estimated Active Implants:	43,000	Without Compromised Therapy:	2
		With Compromised Therapy:	-

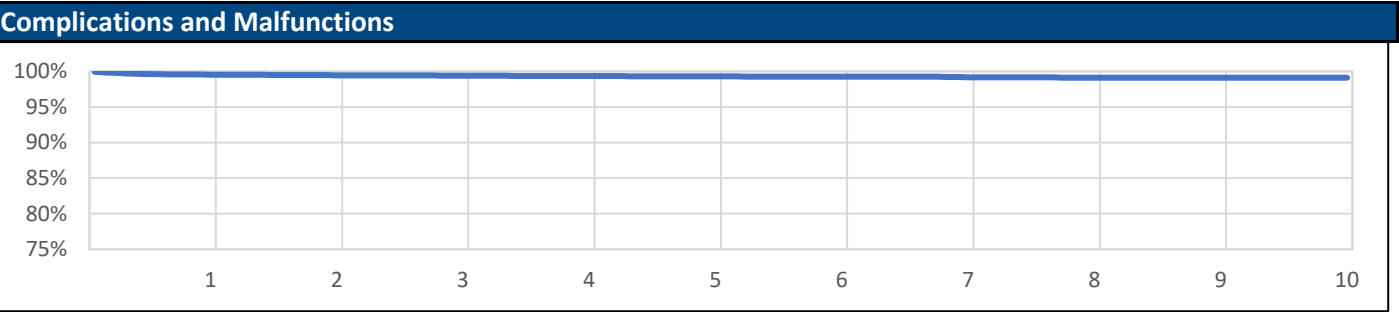

US Survival Probability											
Year		1	2	3	4	5	6	7	8	9	10
Non-Advisory Population	Complications and Malfunctions	99.5%	99.5%	99.4%	99.4%	99.3%	99.2%	99.2%	99.1%	99.1%	99.1%
Registered Implants: 50000	Effective Sample Size	39486	30770	23272	16739	11387	6754	3427	891	358	217

# ACUITY X4 Straight

Models: 4671/4672


Worldwide Confirmed Malfunctions		4	
Worldwide Distribution		112,000	
US Approval Date: February 2016			
	With Compromised Therapy	Without Compromised Therapy	Total
Other			
Non-patterned, other	0	4	4
Grand Total	0	4	4

References cited in table above [\(link\)](#)

# ACUITY Spiral

Models: 4591/4592/4593

US Summary			
US Registered Implants:	24,000	US Chronic Complications	586
US Approval Date:	May 2008	US Malfunctions:	9
US Estimated Active Implants:	12,000	Without Compromised Therapy:	5
		With Compromised Therapy:	4

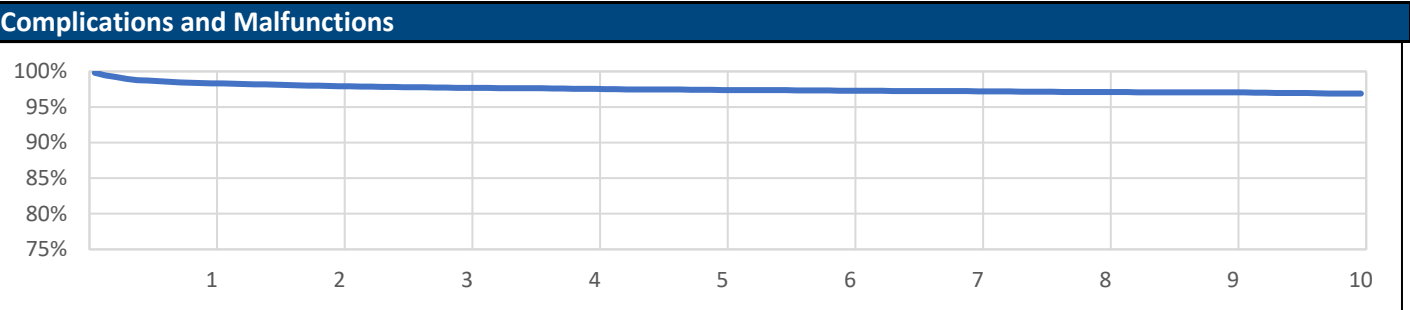

US Survival Probability												
Year		1	2	3	4	5	6	7	8	9	10	
Non-Advisory Population	Complications and Malfunctions	98.3%	97.9%	97.7%	97.5%	97.4%	97.3%	97.2%	97.1%	97.0%	96.9%	
Registered Implants: 24000		Effective Sample Size	20112	17883	15938	14186	12609	11117	9793	8558	7224	5723

# ACUITY Spiral

Models: 4591/4592/4593


Worldwide Confirmed Malfunctions		9	
Worldwide Distribution		47,000	
US Approval Date: May 2008			
	With Compromised Therapy	Without Compromised Therapy	Total
Other			
Non-patterned, other	4	5	9
Grand Total	4	5	9

References cited in table above [\(link\)](#)

# ACUITY Steerable

Models: 4554/4555/4556

US Summary			
US Registered Implants:	29,000	US Chronic Complications	754
US Approval Date:	May 2008	US Malfunctions:	33
US Estimated Active Implants:	12,000	Without Compromised Therapy:	12
		With Compromised Therapy:	21

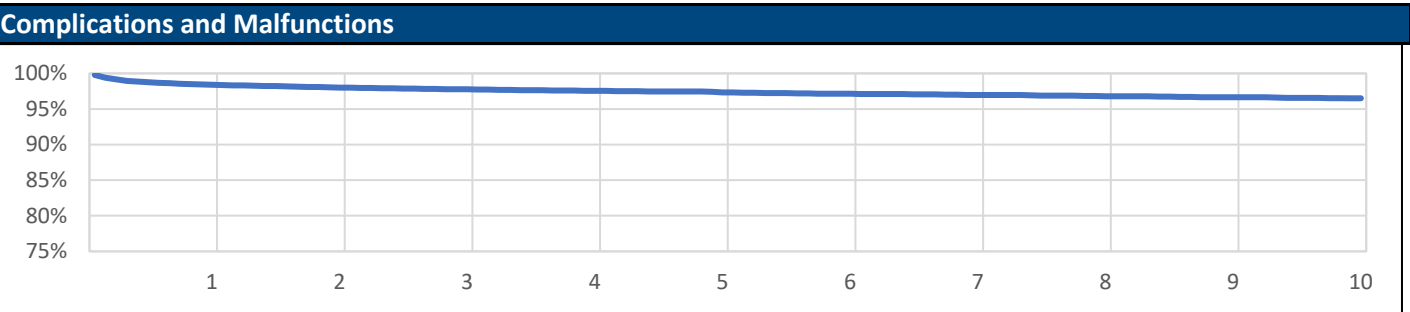

US Survival Probability												
Year		1	2	3	4	5	6	7	8	9	10	
Non-Advisory Population	Complications and Malfunctions	98.4%	98.0%	97.8%	97.6%	97.3%	97.1%	97.0%	96.8%	96.6%	96.5%	
Registered Implants: 29000		Effective Sample Size	24509	21902	19626	17619	15817	14165	12670	11319	9872	8193

# ACUITY Steerable

Models: 4554/4555/4556


Worldwide Confirmed Malfunctions		57	
Worldwide Distribution		65,000	
US Approval Date: May 2008			
	With Compromised Therapy	Without Compromised Therapy	Total
Conductor			
Extracardiac fracture (34)	28	8	36
Other			
Non-patterned, other	10	11	21
Grand Total	38	19	57

References cited in table above [\(link\)](#)

# EASYTRAK 3

Models: 4522/4524/4525/4527/4548/4549/4550

US Summary			
US Registered Implants:	22,000	US Chronic Complications	576
US Approval Date:	August 2004	US Malfunctions:	32
US Estimated Active Implants:	7,000	Without Compromised Therapy:	9
		With Compromised Therapy:	23

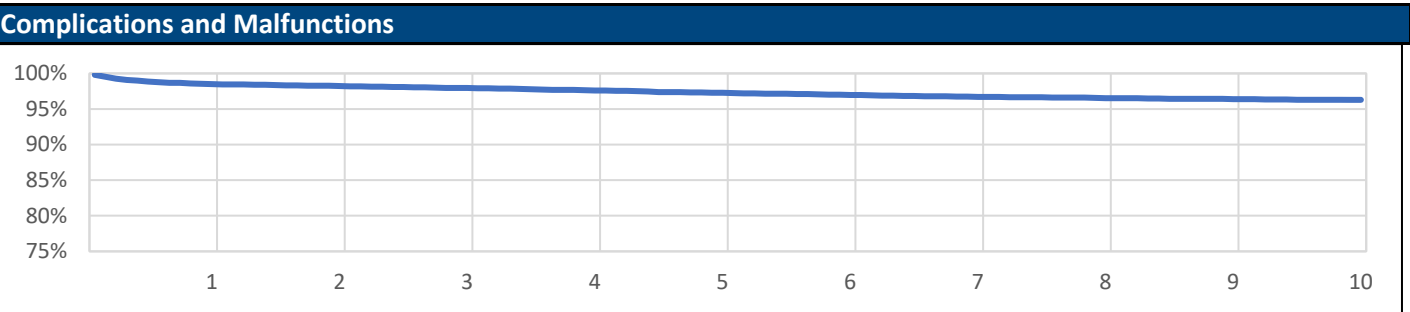

US Survival Probability												
Year		1	2	3	4	5	6	7	8	9	10	
Non-Advisory Population	Complications and Malfunctions	98.5%	98.2%	97.9%	97.6%	97.3%	97.0%	96.7%	96.5%	96.4%	96.3%	
Registered Implants: 22000		Effective Sample Size	18402	16425	14697	13137	11727	10467	9369	8386	7366	6227

# EASYTRAK 3

Models: 4522/4524/4525/4527/4548/4549/4550


Worldwide Confirmed Malfunctions		52	
Worldwide Distribution		43,000	
US Approval Date: August 2004			
	With Compromised Therapy	Without Compromised Therapy	Total
Conductor			
Extracardiac fracture (34)	28	6	34
Other			
Non-patterned, other	7	11	18
Grand Total	35	17	52

References cited in table above [\(link\)](#)

# EASYTRAK 2

Models: 4515/4517/4518/4520/4542/4543/4544

US Summary			
US Registered Implants:	97,000	US Chronic Complications	3,025
US Approval Date:	August 2004	US Malfunctions:	411
US Estimated Active Implants:	31,000	Without Compromised Therapy:	151
		With Compromised Therapy:	260

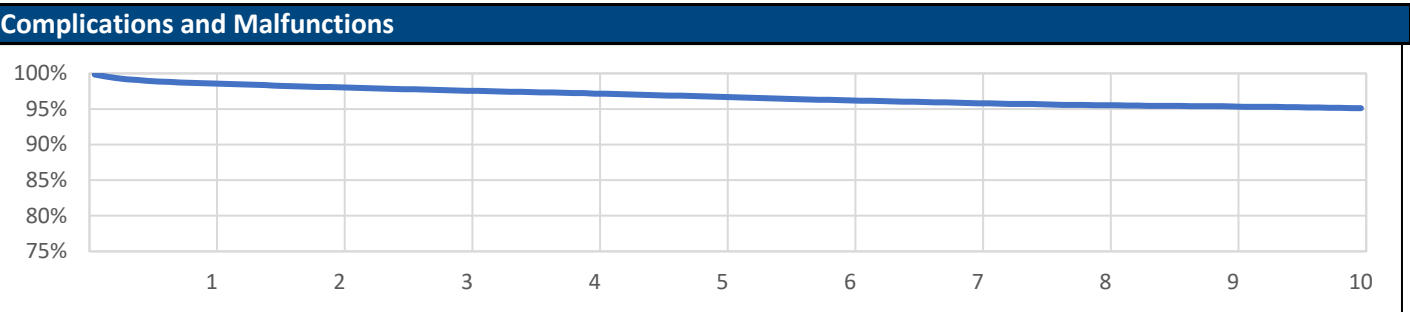

US Survival Probability												
Year		1	2	3	4	5	6	7	8	9	10	
Non-Advisory Population	Complications and Malfunctions	98.6%	98.0%	97.6%	97.2%	96.7%	96.2%	95.8%	95.5%	95.4%	95.1%	
Registered Implants: 97000		Effective Sample Size	82213	73225	65348	58385	52089	46378	41348	36797	32078	27077

# EASYTRAK 2

Models: 4515/4517/4518/4520/4542/4543/4544


Worldwide Confirmed Malfunctions		554	
Worldwide Distribution		180,000	
US Approval Date: August 2004			
	With Compromised Therapy	Without Compromised Therapy	Total
Conductor			
Conductor fracture (25)	329	149	478
Other			
Non-patterned, other	40	36	76
Grand Total	369	185	554

References cited in table above [\(link\)](#)

# ENDOTAK RELIANCE 4-FRONT Dual Coil Active Fixation

Models: 0653/0658/0675/0676/0695/0696

US Summary			
US Registered Implants:	13,000	US Chronic Complications	32
US Approval Date:	May 2018	US Malfunctions:	-
US Estimated Active Implants:	12,000	Without Compromised Therapy:	-
		With Compromised Therapy:	-

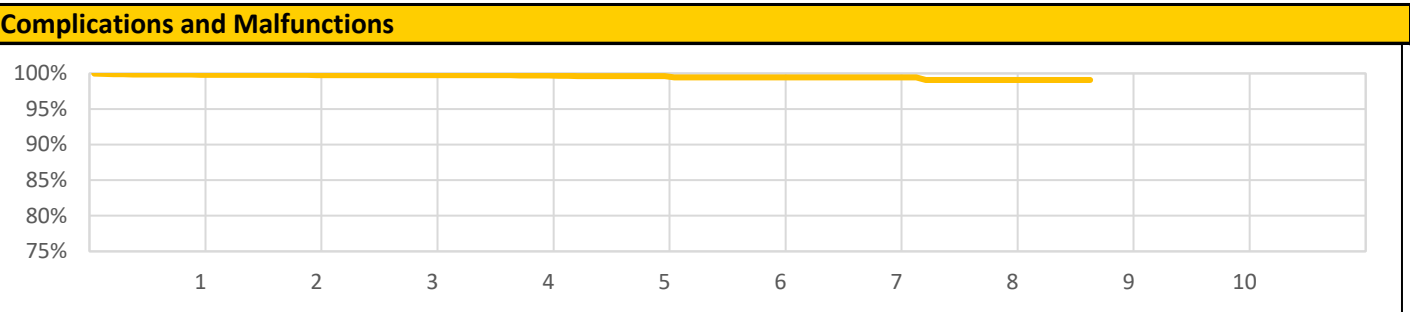

US Survival Probability											
Year		1	2	3	4	5	6	7	8	9	10
Non-Advisory Population	Complications and Malfunctions	99.8%	99.8%	99.7%	99.7%	99.6%	99.5%	99.5%	99.1%	99.1%	--
Registered Implants: 13000	Effective Sample Size	9584	6890	4453	2386	767	299	269	237	200	--

@ 104 months

# ENDOTAK RELIANCE 4-FRONT Dual Coil Active Fixation

Models: 0653/0658/0675/0676/0695/0696

Worldwide Confirmed Malfunctions		5	
Worldwide Distribution		35,000	
US Approval Date: May 2018			
	With Compromised Therapy	Without Compromised Therapy	Total
Other			
Non-patterned, other	5	0	5
Grand Total	5	0	5

References cited in table above [\(link\)](#)

# ENDOTAK RELIANCE 4-FRONT Dual Coil Passive Fixation

Models: 0636/0651/0655/0665/0685/0686


Worldwide Confirmed Malfunctions		0	
Worldwide Distribution		2,000	
US Approval Date: May 2018			
		Without	
		With Compromised	Compromised
		Therapy	Therapy
		Total	
Other			
Non-patterned, other		0	0
Grand Total		0	0

References cited in table above [\(link\)](#)

# ENDOTAK RELIANCE 4-FRONT Single Coil Active Fixation

Models: 0657/0672/0673/0692/0693

US Summary			
US Registered Implants:	99,000	US Chronic Complications	302
US Approval Date:	May 2018	US Malfunctions:	21
US Estimated Active Implants:	92,000	Without Compromised Therapy:	3
		With Compromised Therapy:	18

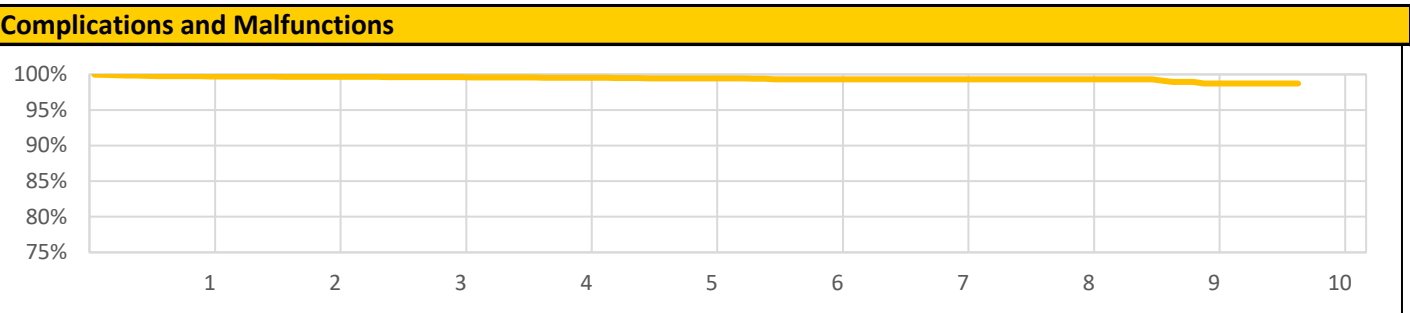

US Survival Probability											
Year		1	2	3	4	5	6	7	8	9	10
Non-Advisory Population	Complications and Malfunctions	99.7%	99.7%	99.6%	99.5%	99.5%	99.3%	99.3%	99.3%	98.7%	98.7%
	Effective Sample Size	68510	46490	29175	14658	4333	799	716	641	410	204
Registered Implants: 99000											

@ 116 months

# ENDOTAK RELIANCE 4-FRONT Single Coil Active Fixation

Models: 0652/ 0657/0672/0673/0692/0693


Worldwide Confirmed Malfunctions		94	
Worldwide Distribution		298,000	
US Approval Date: May 2018			
	With Compromised Therapy	Without Compromised Therapy	Total
Conductor			
Conductor cable fracture (38)	24	0	24
Other			
Non-patterned, other	59	11	70
Grand Total	83	11	94

References cited in table above [\(link\)](#)

# ENDOTAK RELIANCE 4-FRONT Single Coil Passive Fixation

Models: 0650/0654/0662/0663/0682/0683

US Summary			
US Registered Implants:	2,000	US Chronic Complications	2
US Approval Date:	May 2018	US Malfunctions:	-
US Estimated Active Implants:	2,000	Without Compromised Therapy:	-
		With Compromised Therapy:	-

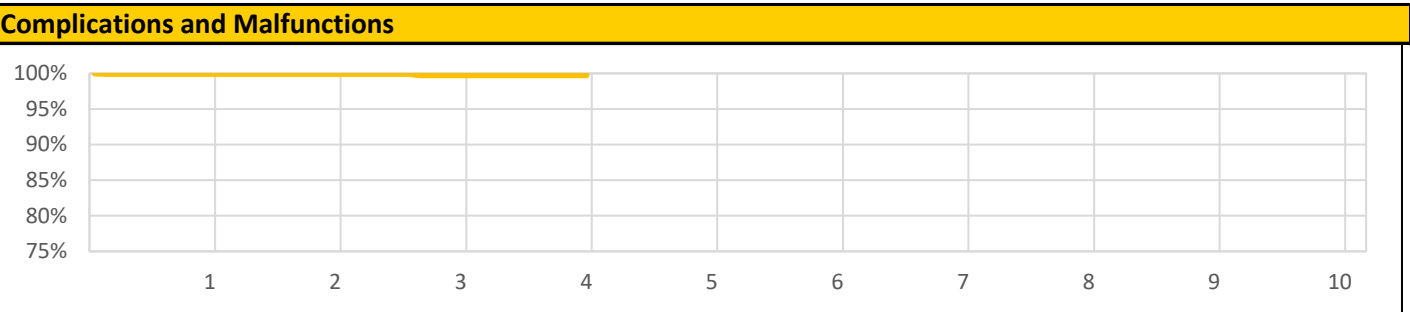

US Survival Probability											
Year		1	2	3	4	5	6	7	8	9	10
Non-Advisory Population	Complications and Malfunctions	99.9%	99.9%	99.7%	99.7%	--	--	--	--	--	--
	Effective Sample Size	1134	714	433	204	--	--	--	--	--	--
Registered Implants: 2000											

@ 48 months

# ENDOTAK RELIANCE 4-FRONT Single Coil Passive Fixation

Models: 0650/0654/0662/0663/0682/0683


Worldwide Confirmed Malfunctions		1	
Worldwide Distribution		9,000	
US Approval Date: May 2018			
	With Compromised Therapy	Without Compromised Therapy	Total
Conductor			
Conductor cable fracture (38)	1	0	1
Grand Total	1	0	1

References cited in table above [\(link\)](#)

# EMBLEM S-ICD Electrode

Models: 3501

US Summary			
US Registered Implants:	37,000	US Chronic Complications	229
US Approval Date:	September 2017	US Malfunctions:	87
US Estimated Active Implants:	33,000	Without Compromised Therapy:	7
		With Compromised Therapy:	80

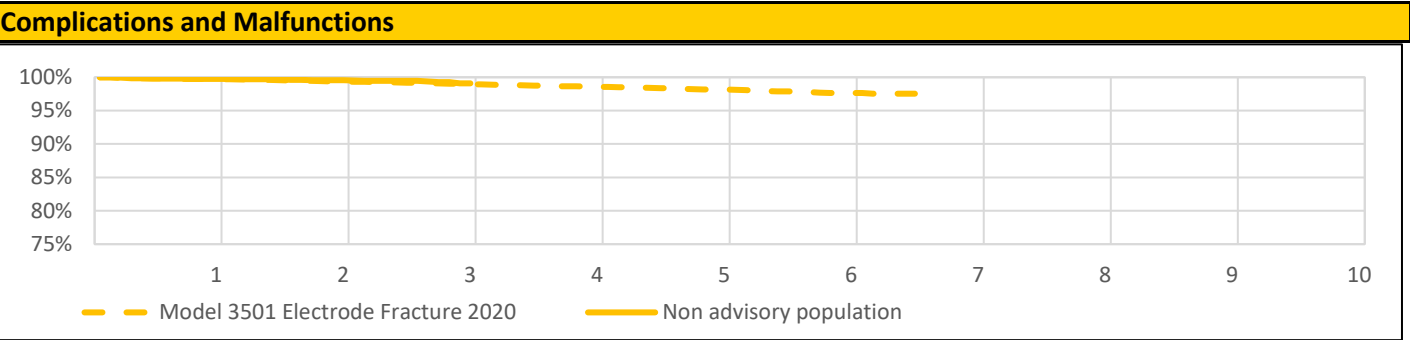

US Survival Probability											
Year		1	2	3	4	5	6	7	8	9	10
Non advisory population	Complications and Malfunctions	99.8%	99.5%	99.1%	--	--	--	--	--	--	--
Registered Implants: 9000	Effective Sample Size	10005	4382	299	--	--	--	--	--	--	--

@ 36 months

\*Devices subject to an advisory. Refer to the Advisories for more details. Devices may be part of more than one advisory.

# EMBLEM S-ICD Electrode

Models: 3501

US Survival Probability (cont.)											
Year		1	2	3	4	5	6	7	8	9	10
Model 3501 Electrode Fracture 2020 Registered Implants: 21000	Complications and Malfunctions	99.7%	99.4%	99.0%	98.6%	98.2%	97.6%	97.5%	--	--	--
	Effective Sample Size	17545	15527	13773	9094	4935	1381	229	--	--	--

@ 78 months

# EMBLEM S-ICD Electrode

Models: 3501


Worldwide Confirmed Malfunctions		232		
Worldwide Distribution		96,000		
US Approval Date: September 2017				
		With Compromised Therapy	Without Compromised Therapy	Total
Conductor				
Model 3501 electrode fracture 2020 (42)		89	2	91
Electrode conductor fracture in or near the pocket (44)		117	15	132
Other				
Non-patterned, other		8	1	9
Grand Total		214	18	232

References cited in table above [\(link\)](#)

# EMBLEM/Q-TRAK S-ICD Electrode

Models: 3010/3401

US Summary			
US Registered Implants:	24,000	US Chronic Complications	237
US Approval Date:	September 2012	US Malfunctions:	36
US Estimated Active Implants:	17,000	Without Compromised Therapy:	8
		With Compromised Therapy:	28

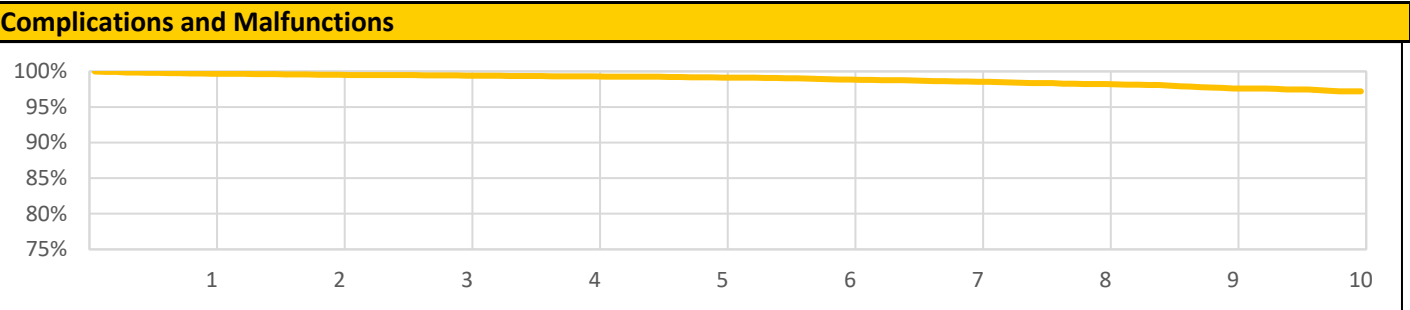

US Survival Probability												
Year		1	2	3	4	5	6	7	8	9	10	
Non-Advisory Population	Complications and Malfunctions	99.7%	99.5%	99.4%	99.3%	99.1%	98.8%	98.6%	98.2%	97.6%	97.2%	
Registered Implants: 24000		Effective Sample Size	21019	18687	16629	14779	13035	11255	8104	4711	2184	752

# EMBLEM/Q-TRAK S-ICD Electrode

Models: 3010/3401


Worldwide Confirmed Malfunctions		96	
Worldwide Distribution		43,000	
US Approval Date: September 2012			
	With Compromised Therapy	Without Compromised Therapy	Total
Conductor			
Electrode conductor fracture in or near the pocket (44)	43	6	49
Crimp/Weld/Bond			
Weld fracture (37)	3	0	3
Other			
Non-patterned, other	30	14	44
Grand Total	76	20	96

References cited in table above [\(link\)](#)

# ENDOTAK RELIANCE 4-Site Dual Coil, Active Fixation

Models: 0275/0276/0295/0296

US Summary			
US Registered Implants:	78,000	US Chronic Complications	474
US Approval Date:	November 2010	US Malfunctions:	33
US Estimated Active Implants:	56,000	Without Compromised Therapy:	7
		With Compromised Therapy:	26

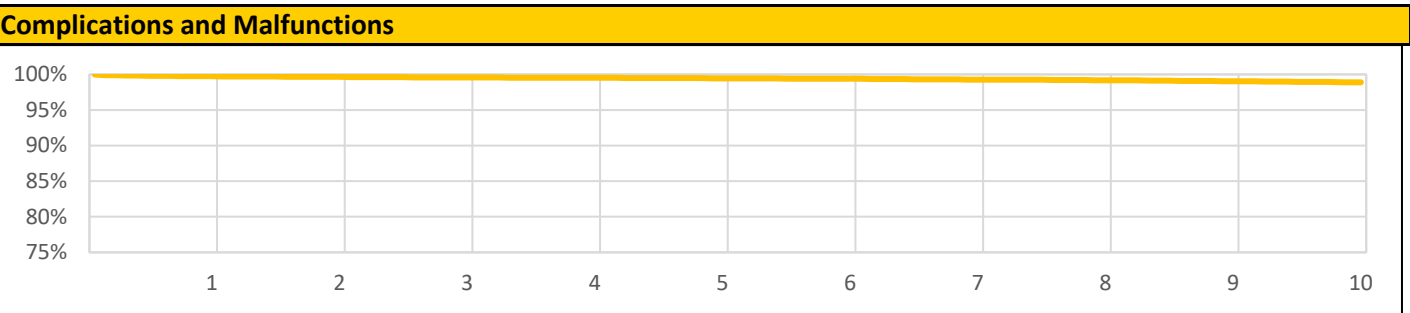

US Survival Probability											
Year		1	2	3	4	5	6	7	8	9	10
Non-Advisory Population	Complications and Malfunctions	99.7%	99.6%	99.6%	99.5%	99.5%	99.4%	99.3%	99.2%	99.0%	98.9%
Registered Implants: 78000	Effective Sample Size	68641	61196	54583	48374	42196	34927	27938	21733	16105	10562

# ENDOTAK RELIANCE 4-Site Dual Coil, Active Fixation

Models: 0275/0276/0295/0296


Worldwide Confirmed Malfunctions		70	
Worldwide Distribution		127,000	
US Approval Date: November 2010			
	With Compromised Therapy	Without Compromised Therapy	Total
Conductor			
Conductor fracture (24)	3	0	3
Other			
Non-patterned, other	53	14	67
Grand Total	56	14	70

References cited in table above [\(link\)](#)

# ENDOTAK RELIANCE 4-Site Dual Coil, Passive Fixation

Models: 0265/0266/0285/0286

US Summary			
US Registered Implants:	3,000	US Chronic Complications	45
US Approval Date:	November 2010	US Malfunctions:	2
US Estimated Active Implants:	3,000	Without Compromised Therapy:	2
		With Compromised Therapy:	-

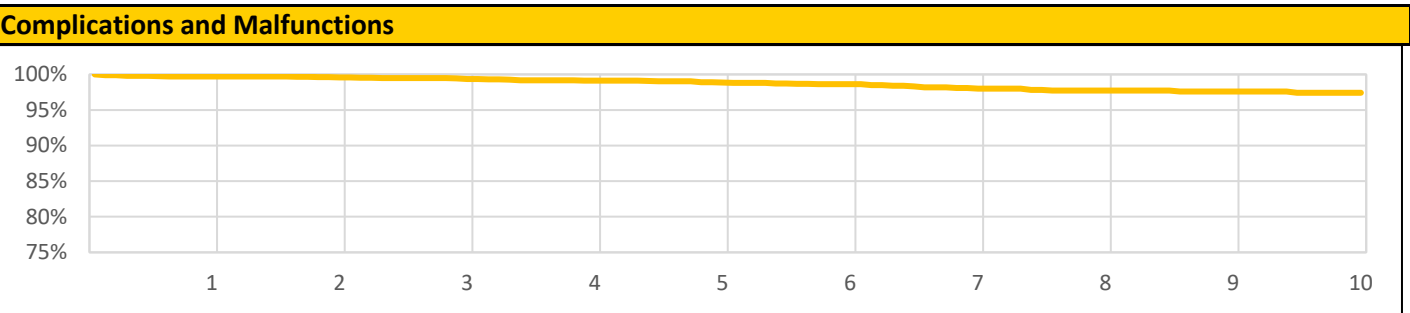

US Survival Probability											
Year		1	2	3	4	5	6	7	8	9	10
Non-Advisory Population	Complications and Malfunctions	99.7%	99.6%	99.3%	99.1%	98.9%	98.6%	98.0%	97.7%	97.6%	97.4%
Registered Implants: 3000	Effective Sample Size	3017	2685	2373	2087	1790	1477	1180	907	668	396

# ENDOTAK RELIANCE 4-Site Dual Coil, Passive Fixation

Models: 0265/0266/0285/0286


Worldwide Confirmed Malfunctions		3	
Worldwide Distribution		11,000	
US Approval Date: November 2010			
	With Compromised Therapy	Without Compromised Therapy	Total
Other			
Non-patterned, other	0	3	3
Grand Total	0	3	3

References cited in table above [\(link\)](#)

# ENDOTAK RELIANCE 4-Site Single Coil, Active Fixation

Models: 0272/0273/0292/0293

US Summary			
US Registered Implants:	120,000	US Chronic Complications	696
US Approval Date:	November 2010	US Malfunctions:	59
US Estimated Active Implants:	94,000	Without Compromised Therapy:	13
		With Compromised Therapy:	46

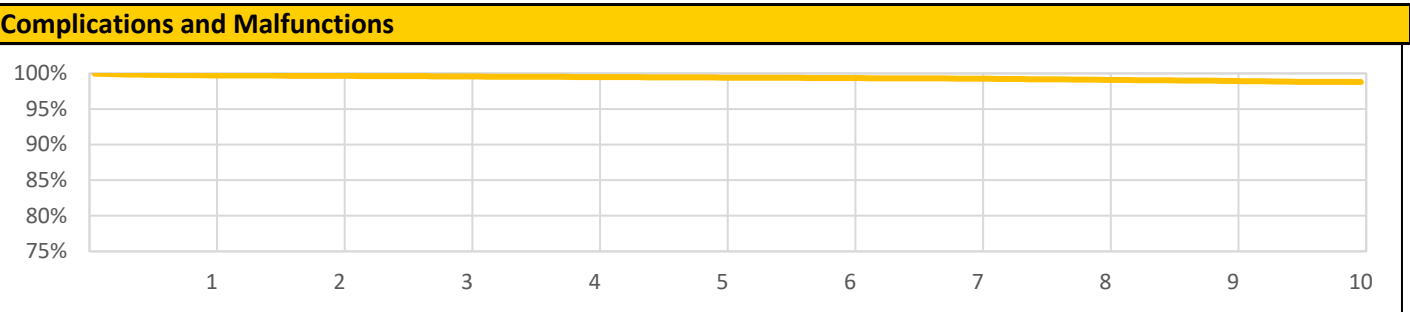

US Survival Probability												
Year		1	2	3	4	5	6	7	8	9	10	
Non-Advisory Population	Complications and Malfunctions	99.7%	99.7%	99.6%	99.5%	99.4%	99.3%	99.3%	99.1%	98.9%	98.8%	
Registered Implants: 120000		Effective Sample Size	105647	94695	84905	75831	66457	50572	34512	22846	13829	7235

# ENDOTAK RELIANCE 4-Site Single Coil, Active Fixation

Models: 0272/0273/0292/0293


Worldwide Confirmed Malfunctions		105	
Worldwide Distribution		217,000	
US Approval Date: November 2010			
	With Compromised Therapy	Without Compromised Therapy	Total
Conductor			
Conductor fracture (24)	12	0	12
Other			
Non-patterned, other	74	19	93
Grand Total	86	19	105

References cited in table above [\(link\)](#)

# ENDOTAK RELIANCE 4-Site Single Coil, Passive Fixation

Models: 0262/0263/0282/0283

US Summary			
US Registered Implants:	25,000	US Chronic Complications	70
US Approval Date:	November 2010	US Malfunctions:	5
US Estimated Active Implants:	23,000	Without Compromised Therapy:	-
		With Compromised Therapy:	5

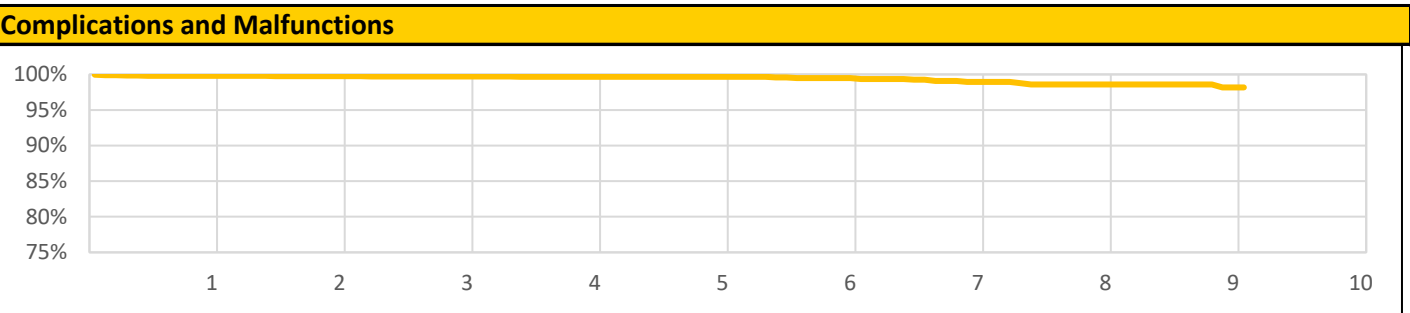

US Survival Probability											
Year		1	2	3	4	5	6	7	8	9	10
Non-Advisory Population	Complications and Malfunctions	99.8%	99.7%	99.7%	99.7%	99.6%	99.5%	99.0%	98.6%	98.2%	98.2%
Registered Implants: 25000	Effective Sample Size	20078	14507	9779	5576	2300	957	631	401	221	202

@ 109 months

# ENDOTAK RELIANCE 4-Site Single Coil, Passive Fixation

Models: 0262/0263/0282/0283


Worldwide Confirmed Malfunctions		10	
Worldwide Distribution		13,000	
US Approval Date: November 2010			
	With Compromised Therapy	Without Compromised Therapy	Total
Other			
Non-patterned, other	9	1	10
Grand Total	9	1	10

References cited in table above [\(link\)](#)

# ENDOTAK RELIANCE Dual Coil, Active Fixation

Models: 0157/0158/0159/0164/0165/0166/0167/0184/0185/0186/0187

US Summary			
US Registered Implants:	287,000	US Chronic Complications	3,851
US Approval Date:	July 2002	US Malfunctions:	398
US Estimated Active Implants:	102,000	Without Compromised Therapy:	128
		With Compromised Therapy:	270

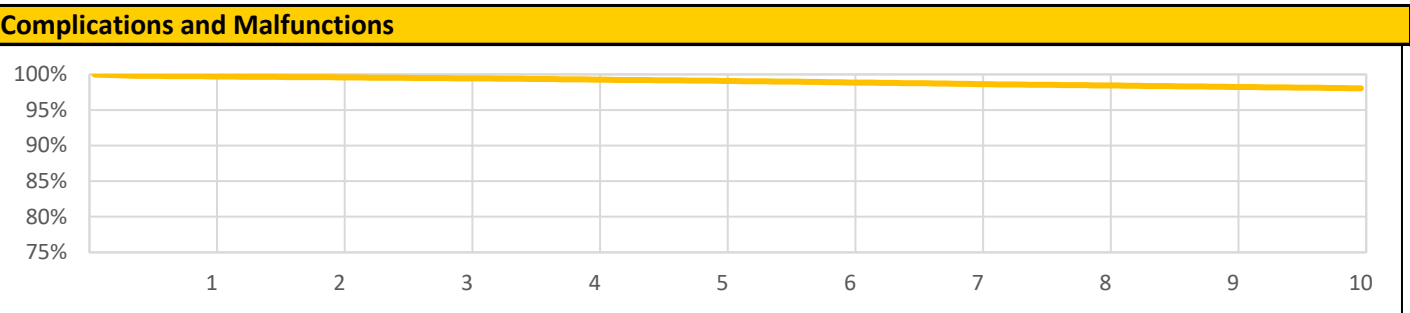

US Survival Probability												
Year		1	2	3	4	5	6	7	8	9	10	
Non-Advisory Population	Complications and Malfunctions	99.7%	99.6%	99.4%	99.3%	99.1%	98.9%	98.6%	98.5%	98.2%	98.1%	
Registered Implants: 287000		Effective Sample Size	252188	226328	203254	182428	163612	146493	131128	117332	104675	93129

# ENDOTAK RELIANCE Dual Coil, Active Fixation

Models: 0157/0158/0159/0164/0165/0166/0167/0184/0185/0186/0187


Worldwide Confirmed Malfunctions		599	
Worldwide Distribution		383,000	
US Approval Date: July 2002			
	With Compromised Therapy	Without Compromised Therapy	Total
Conductor			
Conductor fracture (24)	107	0	107
Crimp/Weld/Bond			
Seal rings (5)	2	2	4
Other			
Non-patterned, other	279	209	488
Grand Total	388	211	599

References cited in table above [\(link\)](#)

# ENDOTAK RELIANCE Single Coil, Active Fixation

Models: 0137/0138/0160/0161/0162/0180/0181/0182

US Summary			
US Registered Implants:	35,000	US Chronic Complications	530
US Approval Date:	October 2000	US Malfunctions:	98
US Estimated Active Implants:	21,000	Without Compromised Therapy:	27
		With Compromised Therapy:	71

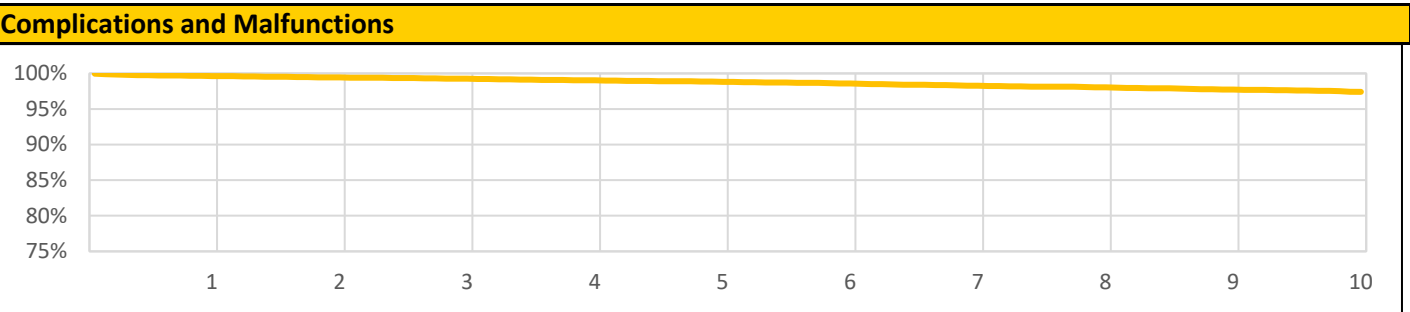

US Survival Probability												
Year		1	2	3	4	5	6	7	8	9	10	
Non-Advisory Population	Complications and Malfunctions	99.6%	99.4%	99.3%	99.0%	98.8%	98.6%	98.3%	98.0%	97.7%	97.4%	
Registered Implants: 35000		Effective Sample Size	30171	26711	23683	20929	18501	16284	14262	12429	10518	8555

# ENDOTAK RELIANCE Single Coil, Active Fixation

Models: 0137/0138/0160/0161/0162/0180/0181/0182


Worldwide Confirmed Malfunctions		222	
Worldwide Distribution		81,000	
US Approval Date: October 2000			
		Without	
		With Compromised	Compromised
		Therapy	Therapy
		Total	
Conductor			
Conductor fracture (24)		62	1
Other			
Non-patterned, other		98	61
Grand Total		160	62
		222	

References cited in table above [\(link\)](#)

# INGEVITY+ Positive Fixation

Models: 7840/7841/7842

US Summary			
US Registered Implants:	397,000	US Chronic Complications	968
US Approval Date:	December 2019	US Malfunctions:	138
US Estimated Active Implants:	372,000	Without Compromised Therapy:	85
		With Compromised Therapy:	53

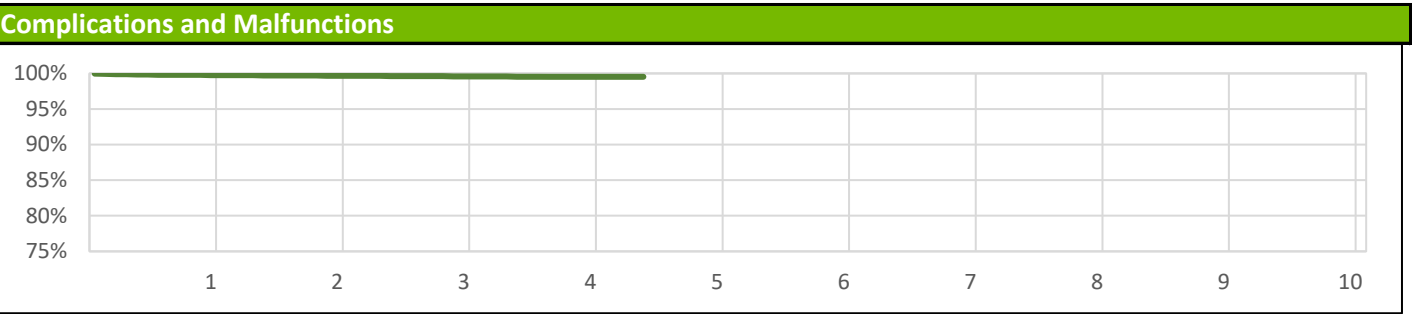

US Survival Probability											
Year		1	2	3	4	5	6	7	8	9	10
Non-Advisory Population	Complications and Malfunctions	99.8%	99.7%	99.6%	99.5%	99.5%	--	--	--	--	--
Registered Implants: 397000	Effective Sample Size	265576	159646	75023	10117	863	--	--	--	--	--

@ 53 months

# INGEVITY+ Positive Fixation

Models: 7840/7841/7842


Worldwide Confirmed Malfunctions	151		
Worldwide Distribution	724,000		
US Approval Date: December 2019			
	With Compromised Therapy	Without Compromised Therapy	Total
Conductor			
Inner conductor break (39)	0	1	1
Extracardiac fracture (41)	21	42	63
Other			
Non-patterned, other	34	48	82
Insulation (43)	0	5	5
Grand Total	55	96	151

References cited in table above [\(link\)](#)

# INGEVITY Positive Fixation

Models: 7640/7641/7642/7740/7741/7742

US Summary			
US Registered Implants:	365,000	US Chronic Complications	2,248
US Approval Date:	April 2016	US Malfunctions:	354
US Estimated Active Implants:	296,000	Without Compromised Therapy:	203
		With Compromised Therapy:	151

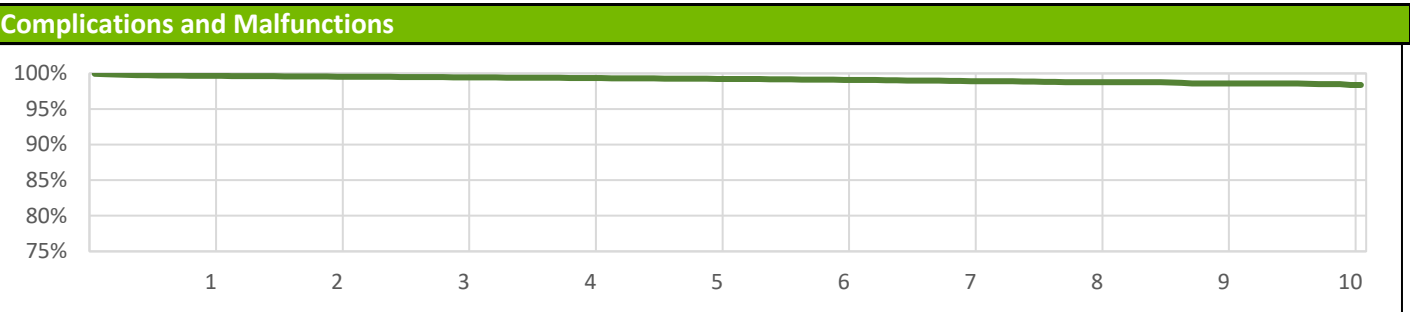

US Survival Probability												
Year		1	2	3	4	5	6	7	8	9	10	
Non-Advisory Population	Complications and Malfunctions	99.7%	99.6%	99.5%	99.3%	99.2%	99.1%	98.9%	98.8%	98.6%	98.4%	
Registered Implants: 365000		Effective Sample Size	321974	288616	258820	230562	164694	99404	46115	4786	1874	1672

# INGEVITY Positive Fixation

Models: 7640/7641/7642/7740/7741/7742


Worldwide Confirmed Malfunctions		522	
Worldwide Distribution		1,120,000	
US Approval Date: April 2016			

References cited in table above [\(link\)](#)

# INGEVITY Atrial J Passive Fixation

Models: 7635/7636/7735/7736

US Summary			
US Registered Implants:	18,000	US Chronic Complications	92
US Approval Date:	April 2016	US Malfunctions:	8
US Estimated Active Implants:	16,000	Without Compromised Therapy:	8
		With Compromised Therapy:	-

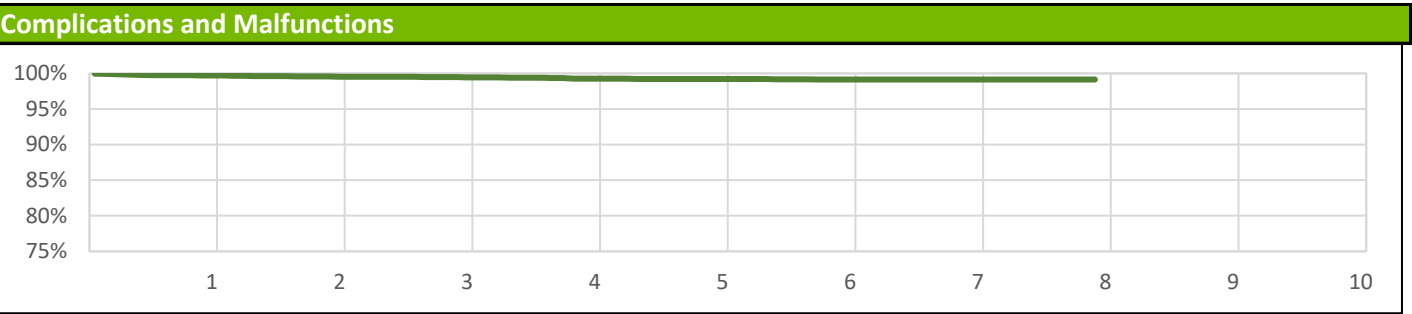

# INGEVITY Atrial J Passive Fixation

Models: 7635/7636/7735/7736


Worldwide Confirmed Malfunctions		15	
Worldwide Distribution		133,000	
US Approval Date: April 2016			
	With Compromised Therapy	Without Compromised Therapy	Total
Conductor			
Extracardiac fracture (41)	0	9	9
Crimp/Weld/Bond			
Weld (40)	0	1	1
Other			
Non-patterned, other	0	5	5
Grand Total	0	15	15

References cited in table above [\(link\)](#)

# INGEVITY Passive Fixation

Models: 7631/7632/7731/7732

US Summary			
US Registered Implants:	31,000	US Chronic Complications	127
US Approval Date:	April 2016	US Malfunctions:	16
US Estimated Active Implants:	26,000	Without Compromised Therapy:	3
		With Compromised Therapy:	13

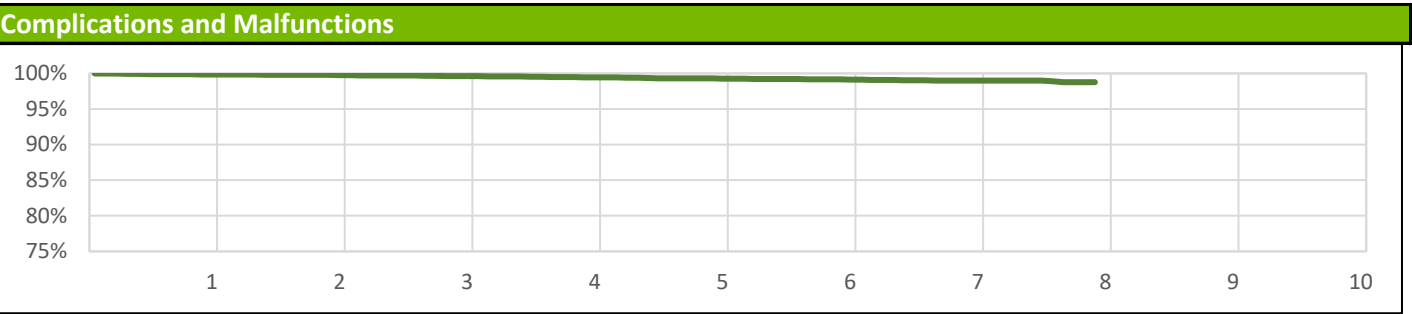

US Survival Probability											
Year		1	2	3	4	5	6	7	8	9	10
Non-Advisory Population	Complications and Malfunctions	99.8%	99.8%	99.6%	99.4%	99.3%	99.1%	99.0%	98.8%	--	--
Registered Implants: 31000	Effective Sample Size	25235	20151	15582	11524	7967	4897	2296	326	--	--

@ 95 months

# INGEVITY Passive Fixation

Models: 7631/7632/7731/7732


Worldwide Confirmed Malfunctions		23	
Worldwide Distribution		139,000	
US Approval Date: April 2016			
	With Compromised Therapy	Without Compromised Therapy	Total
Conductor			
Extracardiac fracture (41)	7	0	7
Other			
Insulation (43)	0	1	1
Non-patterned, other	13	2	15
Grand Total	20	3	23

References cited in table above [\(link\)](#)

# FINELINE II EZ/FINELINE II Sterox EZ Positive Fixation (Polyurethane)

Models: 4463/4464/4465/4469/4470/4471

US Summary			
US Registered Implants:	527,000	US Chronic Complications	3,974
US Approval Date:	January 2000	US Malfunctions:	176
US Estimated Active Implants:	260,000	Without Compromised Therapy:	58
		With Compromised Therapy:	118

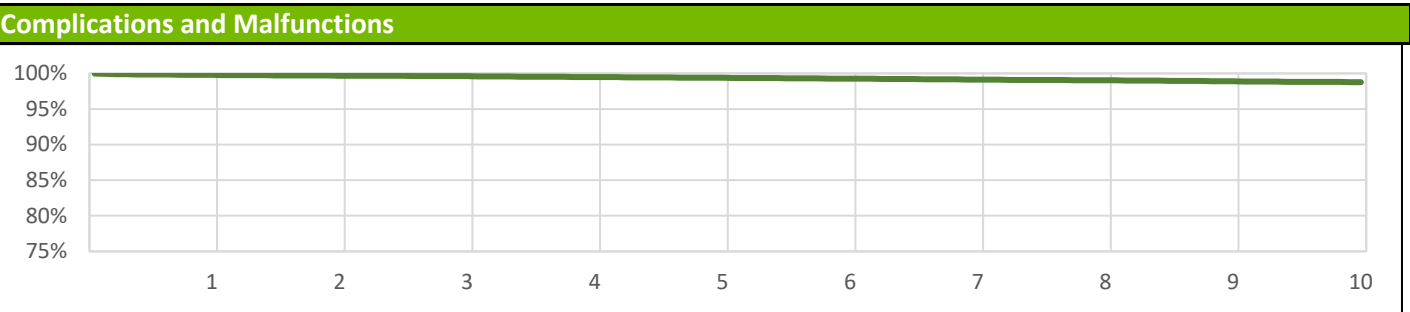

US Survival Probability												
Year		1	2	3	4	5	6	7	8	9	10	
Non-Advisory Population	Complications and Malfunctions	99.8%	99.7%	99.6%	99.5%	99.4%	99.3%	99.1%	99.0%	98.9%	98.8%	
Registered Implants: 527000		Effective Sample Size	458289	404087	356371	313491	273942	237607	205419	177697	147980	120852

# FINELINE II EZ/FINELINE II Sterox EZ Positive Fixation (Polyurethane)

Models: 4463/4464/4465/4469/4470/4471

Worldwide Confirmed Malfunctions	209
Worldwide Distribution	839,000


US Approval Date: January 2000			
	With Compromised Therapy	Without Compromised Therapy	Total
Conductor			
Lead conductor (7)	66	19	85
Crimp/Weld/Bond			
Terminal weld (23)	1	0	1
Other			
Lead body (4)	71	33	104
Non-patterned, other	8	10	18
Insulation (43)	0	1	1
Grand Total	146	63	209

References cited in table above [\(link\)](#)

# FINELINE II/FINELINE II Sterox Atrial J (Polyurethane)

Models: 4477/4478/4479/4480

US Summary			
US Registered Implants:	64,000	US Chronic Complications	859
US Approval Date:	January 2000	US Malfunctions:	39
US Estimated Active Implants:	26,000	Without Compromised Therapy:	20
		With Compromised Therapy:	19

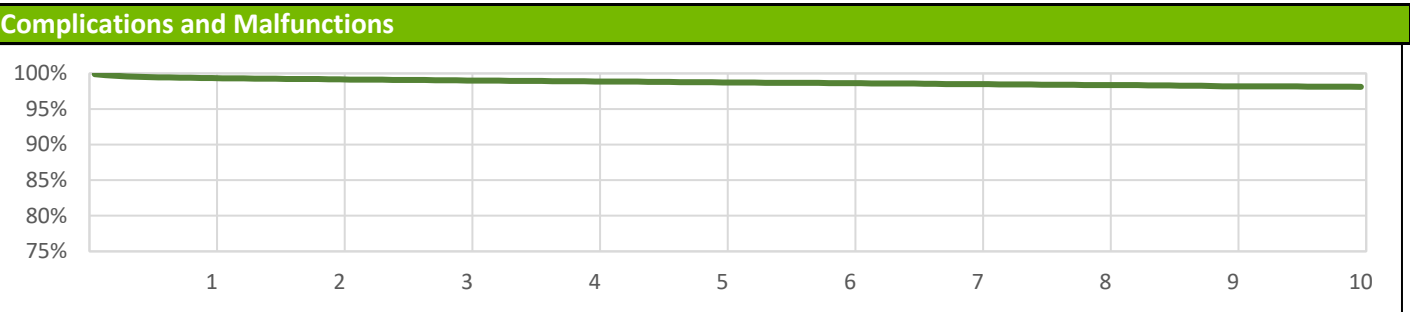

US Survival Probability												
Year		1	2	3	4	5	6	7	8	9	10	
Non-Advisory Population	Complications and Malfunctions	99.3%	99.2%	99.0%	98.9%	98.7%	98.6%	98.5%	98.4%	98.2%	98.1%	
Registered Implants: 64000		Effective Sample Size	55341	49549	44418	39770	35592	31716	28058	24763	20844	17239

# FINELINE II/FINELINE II Sterox Atrial J (Polyurethane)

Models: 4477/4478/4479/4480


Worldwide Confirmed Malfunctions		79	
Worldwide Distribution		330,000	
US Approval Date: January 2000			
	With Compromised Therapy	Without Compromised Therapy	Total
Conductor			
Lead conductor (7)	5	2	7
Other			
J-shape (22)	26	30	56
Lead body (4)	8	3	11
Non-patterned, other	3	2	5
Grand Total	42	37	79

References cited in table above [\(link\)](#)

# FINELINE II/FINELINE II Sterox Passive Fixation (Polyurethane)

Models: 4452/4453/4456/4457

US Summary			
US Registered Implants:	199,000	US Chronic Complications	1,702
US Approval Date:	January 2000	US Malfunctions:	48
US Estimated Active Implants:	74,000	Without Compromised Therapy:	3
		With Compromised Therapy:	45

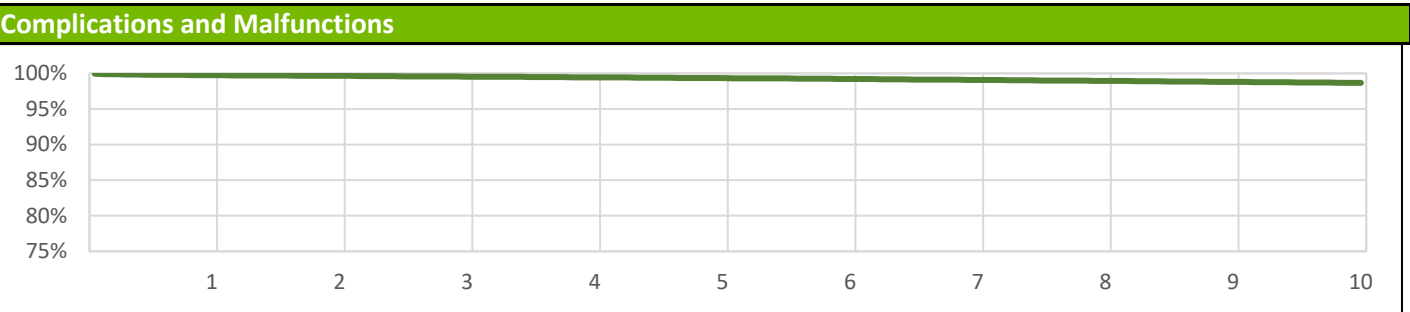

US Survival Probability												
Year		1	2	3	4	5	6	7	8	9	10	
Non-Advisory Population	Complications and Malfunctions	99.7%	99.7%	99.5%	99.4%	99.3%	99.2%	99.1%	99.0%	98.8%	98.7%	
Registered Implants: 199000		Effective Sample Size	171824	153323	136709	121861	108376	95960	84654	74576	63270	52625

# FINELINE II/FINELINE II Sterox Passive Fixation (Polyurethane)

Models: 4452/4453/4456/4457

Worldwide Confirmed Malfunctions		71	
Worldwide Distribution		560,000	
US Approval Date: January 2000			
	With Compromised Therapy	Without Compromised Therapy	Total
Conductor			
Lead conductor (7)	20	0	20
Other			
Lead body (4)	41	3	44
Non-patterned, other	6	1	7
Grand Total	67	4	71

References cited in table above [\(link\)](#)

## Confirmed Malfunction Details: Leads References

Descriptions listed below provide an overview of the clinical observations and/or analysis findings associated with each confirmed lead malfunction pattern listed in this report. All of the patterns listed are thoroughly investigated and analyzed. As part of Boston Scientific's process of continuous improvement, when possible, changes have been or will be implemented in response to identified malfunction patterns. "Improvements implemented" may include product design changes in existing or subsequent generations, manufacturing process modifications, educational communications, labeling changes, etc. Improvement implementation may vary by geography due to various factors, including regulatory review timing, and may not completely mitigate or eliminate the potential for additional malfunctions.

1. **IS-1 terminal pin**— Compromised insulation and/or conductor integrity if lead is bent sharply away from the header block when placed in implant pocket or if pulse generator migrates from implant site. Improvement implemented.
2. **Inner insulation abrasion**— Loss of capture, decreasing impedance, increased pacing thresholds, noisy signals, oversensing. Abrasion of inner insulation.
3. **Terminal leg insulation**— Loss of sensing, loss of pacing, loss of defibrillation therapy. Abraded insulation on terminal leg portion of lead due to lead-on-lead or lead-on-can contact. Improvement implemented.
4. **Lead body**— Insulation abrasion due to lead-on-lead or lead-on-can contact combined with damage attributed to application of compressive or torsional loads which may be due to clavicle-first rib entrapment. Damage to lead body may expose conductor.
5. **Seal rings**— Insertion difficulty at implant, difficulty removing lead from header post-implant. Proximal silicone seal rings not fully adhered to lead terminal. Improvement implemented.
6. **Manufacturing material**— Loss of sensing, loss of pacing, noisy signals. Manufacturing material embedded in lead body.
7. **Lead conductor**— Loss of capture, inability to deliver therapy. Fatigue of lead conductor due to repeated flexing.
8. **Lead body**— Lead fracture, inappropriate shocks, oversensing. Insulation damage resulting from implant stresses or manufacturing variability.
9. **Lead conductor**— Loss of sensing, loss of pacing. Physical damage to lead body due to repeated flexing.
10. **Lead connector**— Insulation damage resulting from bending or tension at the terminal connector. May lead to inappropriate shocks, oversensing.
11. **Lead conductor**— Physical damage to lead conductor, inappropriate shocks, oversensing. Displacement of yoke component may lead to fatigue of high-voltage lead conductor. Improvement implemented.
12. **Conductor connection**— Loss of sensing, loss of pacing, loss of defibrillation output. Improper conductor wire connection. Improvement implemented.
13. **Serial number label**— Loss of sensing, loss of pacing. Sharp edge in serial number label resulting in breach in outer lead insulation. Improvement implemented.
14. **Terminal component**— Loss of sensing, loss of pacing, terminal pin separation from terminal ring during implant or ICD replacement. Improvement implemented.
15. **Electrode tip**— Separation between electrode tip and lead body.
16. **Lead body**— Physical damage to lead body, inappropriate shocks. Abraded insulation due to contact with patient anatomy.
17. **DF-1 terminal pin**— Loss of sensing, loss of pacing, loss of defibrillation output. Compromised insulation and/or conductor integrity from sharp or excessive bending. Improvement implemented.
18. **Yoke component**— Noise, impedance anomalies, threshold variation. Use of multiple or pre-formed stylets may cause component within lead yoke to dislodge. Improvement implemented.
19. **Lead conductor**— Muscle stimulation, inappropriate shocks, oversensing, high pacing impedance, inability to deliver therapy. Repeated flexing leading to fatigue of lead conductor.
20. **Serial number label**— Loss of sensing, loss of pacing. Broken serial number label due to either sharp bend away from header at implant or repetitive movement during implant.
21. **IS-1 terminal pin**— Compromised insulation and/or conductor integrity if lead is bent sharply away from the header block when placed in implant pocket or if pulse generator migrates from implant site. Improvement implemented.
22. **J-shape**— Placement difficulty, dislodgement. Elevated temperatures resulting in a relaxation of pre-formed J-shape. Improvement implemented.
23. **Terminal weld**— Impedance rise, loss of pacing. Loss of connection on terminal weld. Improvement implemented.
24. **Conductor fracture**— High impedance, loss of capture, loss of pacing, inappropriate shocks. Flex fatigue leading to discontinuity of pace/sense conductor.
25. **Conductor fracture**— High impedance, loss of LV capture, loss of LV pacing. Flex fatigue leading to discontinuity of conductor.
26. **Non-patterned, Other**— Confirmed malfunction for which the root cause does not fit within other categories and is not associated with other malfunctions, or has not yet been identified.
32. **Conductor damage**— Noise, oversensing, inappropriate shocks, possible loss of therapy. Conductor damage attributed to application of compressive or torsional loads which may be due to clavicle-first rib entrapment.
33. **Insulation damage**— Low pacing impedance, noise, possible loss of therapy. Insulation abrasion due to lead-onlead or lead-on-can contact, or due to application of compressive or torsional loads which may be due to clavicle first rib entrapment. Damage to lead body may expose conductor.

34. **Extracardiac fracture**— High impedance, loss of LV capture, loss of LV pacing. Flex fatigue near suture sleeve, not including clavicle-first rib damage, leading to discontinuity of conductor.
35. **Lead conductor**— High impedance, loss of sensing, loss of pacing. Variability in wire conductor material. Improvement implemented.
36. **Conductor connection**— Loss of sensing, loss of pacing, loss of defibrillation output. Improper conductor wire connection. Improvement implemented.
37. **Weld fracture**— Noise, loss of sensing. Fractured weld.
38. **Conductor cable fracture**— High impedance, potential loss of pacing and defibrillation therapy. Fractured high voltage cable. Improvement implemented.
39. **Inner conductor break**— High impedance, loss of capture, loss of sensing. Inner conductor break. Commonly associated with helix extension/retraction difficulties at implant.
40. **Weld**— Out of range impedance measurements, noise, oversensing. Incomplete weld.
41. **Extracardiac fracture**— High impedance, noise, oversensing, loss of capture, loss of pacing. Flex fatigue leading to discontinuity of outer conductor.
42. **Model 3501 electrode fracture 2020**— *December 2020 Voluntary Physician Advisory*. High shock impedance, loss of tachy therapy. Fractured electrode conductor immediately distal to the proximal sense electrode. Note: per ISO 5841-2:2(E), only returned and confirmed failures are included in this table. All failures associated with this pattern – including reports that are not returned - are included in rate calculations and projections updated in the advisory section.
43. **Insulation**— High pacing impedance, noise, undersensing. Insulation issue.
44. **Electrode conductor fracture in or near pocket**— High shock impedance, loss of tachy therapy. Fractured electrode conductor proximal to the proximal sense electrode.

## U.S. Chronic Lead Complications (Occurring After the First Month of Service)

Boston Scientific strives to provide meaningful detail in describing the performance of our products. U.S. Chronic Lead Complications are reported in compliance with ISO 5841-2: 2014 (E), Reporting of Clinical Performance of Populations of Pulse Generators or Leads. To be included in the Chronic Lead Complications table, a lead must be successfully implanted, with clinical observations (as listed in the table) occurring after the first month of implant, and have been removed from service surgically or electronically. The lead either was not returned for analysis, or was returned but had no confirmation of a malfunction.

While multiple complications are possible for any given lead, only one complication is reported per lead. The complication reported is determined by an observation hierarchy, indicated by the order of the categories from left to right in the table. The number of U.S. Registered Implants is also provided as context for the data. Chronic Lead Complications are included in the calculation of survival probability.

Pacing Leads/Model	U.S. Registered Implants	Cardiac Perforation	Conductor fracture/ helix damage	Lead dislodgement	Failure to capture	Oversensing	Failure to sense	Insulation breach	Abnormal pacing impedance	Abnormal defibrillation impedance	Extracardiac stimulation
INGEVITY+ Positive Fixation 7840/7841/7842	396,000	116	154	497	109	24	16	4	46	0	2
INGEVITY Positive Fixation 7640/7641/7642/7740/7741/7742	365,000	151	754	607	293	143	30	62	183	0	25
INGEVITY Atrial J Passive Fixation 7635/7636/7735/7736	18,000	0	21	47	12	3	2	2	5	0	0
INGEVITY Passive Fixation 7631/7632/7731/7732	31,000	2	43	19	27	8	3	3	22	0	0
FINELINE II ; Passive Fixation (poly) 4452/4453/4456/4457	199,000	5	502	251	312	80	36	218	279	0	19
FINELINE II EZ ; Positive Fixation (poly) 4463/4464/4465/4469/4470/4471	527,000	27	871	927	553	216	165	617	567	0	31
FINELINE II Atrial J (poly) 4477/4478/4479/4480	64,000	2	132	369	144	31	36	82	55	0	8
FINELINE II/THINLINE II ; Passive Fixation (silicone) 4454/4455/4458/4459	14,000	2	130	20	73	30	5	24	41	0	1
FINELINE II/THINLINE II EZ ; Positive Fixation (silicone) 4466/4467/4468/4472/5573/4474	53,000	0	323	97	125	111	26	108	155	0	3
CRT Leads/Model	U.S. Registered Implants	Cardiac Perforation	Conductor fracture/ helix damage	Lead dislodgement	Failure to capture	Oversensing	Failure to sense	Insulation breach	Abnormal pacing impedance	Abnormal defibrillation impedance	Extracardiac stimulation
ACUITY X4 Spiral L 4677/4678	22,000	1	0	36	10	1	0	0	1	0	8
ACUITY X4 Spiral S 4674/4675	67,000	1	2	112	16	2	0	1	1	0	18

<b>CRT Leads/Model (cont.)</b>	U.S. Registered Implants	Cardiac Perforation	Conductor fracture/ helix damage	Lead dislodgement	Failure to capture	Oversensing	Failure to sense	Insulation breach	Abnormal pacing impedance	Abnormal defibrillation impedance	Extracardiac stimulation
ACUITY X4 Straight 4671/4672	50,000	1	2	182	33	1	0	1	6	0	54
ACUITY Steerable 4554/4555/4556	29,000	5	46	465	71	6	2	19	42	0	98
ACUITY Spiral 4591/4592/4593	24,000	0	28	344	57	0	1	5	13	0	138
EASYTRAK 3 4522/4524/4525/4527/4548/4549/4550	22,000	2	48	316	67	5	2	16	25	0	95
EASYTRAK 2 4515/4517/4518/4520/4542/4543/4544	97,000	2	461	1381	396	15	8	119	193	0	450
EASYTRAK 4510/4511/4512/4513/4535/4536/ 4537/4538	38,000	2	92	489	152	4	1	78	55	0	269

<b>Defibrillation Leads/Model</b>	U.S. Registered Implants	Cardiac Perforation	Conductor fracture/ helix damage	Lead dislodgement	Failure to capture	Oversensing	Failure to sense	Insulation breach	Abnormal pacing impedance	Abnormal defibrillation impedance	Extracardiac stimulation
ENDOTAK RELIANCE 4-FRONT Single Coil Active Fixation 0652/0657/0672/0673/0692/0693	99,000	35	49	132	34	22	8	0	11	8	3
ENDOTAK RELIANCE 4-FRONT Dual Coil Active Fixation 0653/0658/0675/0676/0695/0696	13,000	3	3	16	3	3	0	1	0	2	1
ENDOTAK RELIANCE 4-Site ; Dual Coil, Active Fixation 0275/0276/0295/0296	78,000	26	66	125	40	89	16	19	35	51	7
ENDOTAK RELIANCE 4-Site ; Dual Coil, Passive Fixation 0285/0286	3,000	1	4	9	4	9	0	0	15	2	1
ENDOTAK RELIANCE 4-Site ; Single Coil, Active Fixation 0292/0293	141,000	39	102	218	77	119	26	18	64	68	12
ENDOTAK RELIANCE 4-Site ; Single Coil, Passive Fixation 0282/0283	3,000	2	5	3	5	1	0	0	6	1	0
ENDOTAK RELIANCE ; Dual Coil, Active Fixation 0157/0158/0159/0164/0165/0167/ 0184/0185/0186/0187	287,000	35	834	439	255	922	106	170	481	579	30
ENDOTAK RELIANCE ; Dual Coil, Passive Fixation 0147/0148/0149/0174/0175/0176/0177	47,000	6	169	76	86	165	13	48	280	84	7
ENDOTAK RELIANCE ; Single Coil, Active Fixation 0137/0138/0160/0161/0162/0180/0181/0182	35,000	15	125	63	39	92	4	9	67	112	4
ENDOTAK RELIANCE ; Single Coil, Passive Fixation 0127/0128/0170/0171/0172/0173	2,000	0	7	5	3	8	0	1	11	5	0

<b>S-ICD Electrodes/Model</b>	U.S. Registered Implants	Perforation	Conductor fracture	Lead dislodgement	Failure to capture	Oversensing	Failure to sense	Insulation breach	Abnormal defibrillation impedance	Extracardiac stimulation
EMBLEM S-ICD Electrode 3501	37,000	0	11	11	0	178	9	1	4	15
EMBLEM/Q-TRAK S-ICD Electrode 3010, 3401	24,000	0	9	26	0	163	17	4	1	17

## U.S. Acute Lead Observations

Boston Scientific strives to provide meaningful detail reflective of real-world product experience. In the first weeks following lead implantation, physiologic responses and lead performance can vary until chronic lead stability is attained. Acute lead performance may be subject to a number of factors, including patient-specific anatomy, clinical conditions and/or varying implant conditions/techniques.

Because acute implant time contributes to overall clinical experience, Boston Scientific provides specific information regarding acute lead performance. To be included in the Acute Lead Observations table, a lead must first be successfully implanted, with clinical observations occurring within the first month of implant. These reports may or may not have resulted in clinical action and/or product return to Boston Scientific. The categories are consistent with the AdvaMed guidance for *Uniform Reporting of Clinical Performance of Cardiac Rhythm Management Pulse Generators and Leads*. Although multiple observations are possible for any given lead, only one observation is reported per lead. The observation reported is determined by an observation hierarchy, indicated by the order of the categories from left to right in the table. The number of U.S. Registered Implants is also provided as context for the data. Acute Lead Observations are not included in calculation of lead survival probability.

Pacing Leads/Model	U.S. Registered Implants	Cardiac Perforation	Conductor fracture/ helix damage	Lead dislodgement	Failure to capture	Oversensing	Failure to sense	Insulation breach	Abnormal pacing impedance	Abnormal defibrillation impedance	Extracardiac stimulation
INGEVITY+ Positive Fixation 7840/7841/7842	396,000	446	54	1031	255	63	60	4	36	0	6
INGEVITY Positive Fixation 7640/7641/7642/7740/7741/7742	365,000	457	421	944	220	77	50	8	51	0	31
INGEVITY Atrial J Passive Fixation 7635/7636/7735/7736	18,000	1	0	45	11	1	1	0	1	0	0
INGEVITY Passive Fixation 7631/7632/7731/7732	31,000	2	0	47	13	0	3	0	0	0	0
FINELINE II ; Passive Fixation (poly) 4452/4453/4456/4457	199,000	9	11	404	103	7	12	16	15	0	10
FINELINE II Atrial J (poly) 4477/4478/4479/4480	64,000	0	10	398	52	2	16	5	7	0	5
FINELINE II EZ ; Positive Fixation (poly) 4463/4464/4465/4469/4470/4471	527,000	57	50	721	153	89	72	29	82	0	26
FINELINE II/THINLINE II ; Passive Fixation (silicone) 4454/4455/4458/4459	14,000	0	1	28	10	0	0	3	4	0	0
FINELINE II/THINLINE II EZ ; Positive Fixation (silicone) 4466/4467/4468/4472/4473/4474	53,000	2	13	90	13	3	8	6	4	0	3

CRT Leads/Model	U.S. Registered Implants	Cardiac Perforation	Conductor fracture/ helix damage	Lead dislodgement	Failure to capture	Oversensing	Failure to sense	Insulation breach	Abnormal pacing impedance	Abnormal defibrillation impedance	Extracardiac stimulation
ACUITY X4 Spiral L 4677/4678	22,000	0	0	39	51	9	0	0	10	0	21
ACUITY X4 Spiral S 4674/4675	67,000	0	2	93	80	11	0	0	28	0	57

<b>CRT Leads/Model (cont.)</b>	U.S. Registered Implants	Cardiac Perforation	Conductor fracture/ helix damage	Lead dislodgement	Failure to capture	Oversensing	Failure to sense	Insulation breach	Abnormal pacing impedance	Abnormal defibrillation impedance	Extracardiac stimulation
ACUITY X4 Straight 4671/4672	50,000	2	0	184	53	8	1	0	15	0	59
ACUITY Steerable 4554/4555/4556	29,000	1	1	291	22	13	1	1	21	0	162
ACUITY Spiral 4591/4592/4593	24,000	1	2	174	29	5	0	3	9	0	167
EASYTRAK 3 4522/4524/4525/4527/4548/4549/4550	22,000	0	1	240	23	8	1	3	17	0	128
EASYTRAK 2 4515/4517/4518/4520/4542/4543/4544	97,000	7	4	807	84	30	4	14	64	0	510
EASYTRAK 4510/4511/4512/4513/4535/4536/ 4537/4538	38,000	4	4	168	24	11	1	10	20	0	141

<b>Defibrillation Leads/Model</b>	U.S. Registered Implants	Cardiac Perforation	Conductor fracture/ helix damage	Lead dislodgement	Failure to capture	Oversensing	Failure to sense	Insulation breach	Abnormal pacing impedance	Abnormal defibrillation impedance	Extracardiac stimulation
ENDOTAK RELIANCE 4-FRONT Single Coil Active Fixation 0652/0657/0672/0673/0692/0693	99,000	89	18	216	39	24	4	2	15	5	3
ENDOTAK RELIANCE 4-FRONT Dual Coil Active Fixation 0653/0658/0675/0676/0695/0696	13,000	10	1	31	10	3	0	0	2	2	0
ENDOTAK RELIANCE 4-Site ; Dual Coil, Active Fixation 0275/0276/0295/0296	78,000	56	18	253	42	29	3	2	27	7	6
ENDOTAK RELIANCE 4-Site ; Dual Coil, Passive Fixation 0285/0286	3,000	2	0	10	1	0	0	0	4	0	0
ENDOTAK RELIANCE 4-Site ; Single Coil, Active Fixation 0292/0293	141,000	101	20	371	72	59	16	6	32	14	21
ENDOTAK RELIANCE 4-Site ; Single Coil, Passive Fixation 0282/0283	3,000	4	1	6	0	1	1	0	8	0	0
ENDOTAK RELIANCE ; Dual Coil, Active Fixation 0157/0158/0159/0164/0165/0167/ 0184/0185/0186/0187	287,000	82	138	510	130	223	12	17	178	108	44
ENDOTAK RELIANCE ; Dual Coil, Passive Fixation 0147/0148/0149/0174/0175/0176/0177	47,000	5	4	92	36	41	4	3	47	5	0
ENDOTAK RELIANCE ; Single Coil, Active Fixation	35,000	31	7	71	15	20	3	2	18	25	9

0137/0138/0160/0161/0162/0180/0181/0182										
ENDOTAK RELIANCE ; Single Coil, Passive Fixation	2,000	0	0	3	1	2	0	0	1	0
0127/0128/0170/0171/0172/0173										

S-ICD Electrodes/Model	U.S. Registered Implants	Perforation	Conductor fracture	Lead dislodgement	Failure to capture	Oversensing	Failure to sense	Insulation breach	Abnormal defibrillation impedance	Extracardiac stimulation
EMBLEM S-ICD Electrode 3501	37,000	1	2	34	0	326	11	0	5	12
EMBLEM/Q-TRAK S-ICD Electrode 3010/3401	24,000	1	0	21	0	208	6	1	0	15

# Before/During Implant Procedure - Worldwide Malfunctions: Leads

This section of the report depicts the number of product malfunctions that occurred worldwide either before implant (prior to opening the sterile product packaging) or during implant (once the sterile product packaging has been opened). In all cases, the product in question must be returned to Boston Scientific CRM and confirmed through laboratory analysis to have operated or exhibited a problem outside the specified performance limits established by Boston Scientific. Damage incurred during shipping/transit or due to external factors warned against in labeling is not reported as device malfunction here.

The Conductor category includes any conductor break or damage with complete or intermittent loss of continuity that could interrupt current flow, including clavicle fatigue or crush damage. The Insulation category includes any lead insulation breach, such as damage due to lead-on-lead or lead-on-anatomy contact, or clavicle fatigue or crush. The Crimp/Weld/Bond category includes any interruption in the conductor or lead body associated with a point of connection. The Other category includes malfunctions for which the root cause does not fit within other categories or has not yet been determined. The Labeling and Packaging categories include product identification issues and damage to sterile packaging, respectively. The Implant Accessory category includes lead malfunctions due to catheter, guidewire or sheath issues.

CRT Leads/Model	Worldwide Distribution	Conductor	Insulation	Crimp/Weld/Bond	Other	Labeling	Packaging	Implant Accessory
ACUITY X4 Spiral L 4677/4678	54,000	0	0	0	3	0	0	0
ACUITY X4 Spiral S 4674/4675	143,000	0	0	0	5	0	0	0
ACUITY X4 Straight 4671/4672	112,000	0	0	0	0	0	0	0
ACUITY Steerable 4554/4555/4556	65,000	0	0	0	5	0	2	0
ACUITY Spiral 4591/4592/4593	47,000	0	0	0	2	1	0	0

Defibrillation Leads/Model	Worldwide Distribution	Conductor	Insulation	Crimp/Weld/Bond	Other	Labeling	Packaging	Implant Accessory
ENDOTAK RELIANCE 4-FRONT Dual Coil Active Fixation 0653/0658/0675/0676/0695/0696	35,000	0	0	0	8	0	0	0
ENDOTAK RELIANCE 4-FRONT Single Coil Active Fixation 0652/0657/0672/0673/0692/0693	298,000	3	1	0	107	0	0	0
ENDOTAK RELIANCE 4-FRONT Dual Coil Passive Fixation 0636/0651/0655/0665/0685/0686	2,000	0	0	0	0	0	0	0
ENDOTAK RELIANCE 4-FRONT Single Coil Passive Fixation 0650/0654/0662/0682/0663/0683	9,000	0	1	0	0	0	0	0
ENDOTAK RELIANCE 4-Site ; Dual Coil, Active Fixation 0275/0276/0295/0296	127,000	0	0	0	91	0	1	0
ENDOTAK RELIANCE 4-Site ; Dual Coil, Passive Fixation 0265/0266/0285/0286	11,000	0	0	0	7	15	1	0
ENDOTAK RELIANCE 4-Site ; Single Coil, Active Fixation 0292/0293	217,000	0	0	0	67	0	1	0
ENDOTAK RELIANCE 4-Site ; Single Coil, Passive Fixation 0282/0283	7,000	0	0	0	0	0	0	0
ENDOTAK RELIANCE ; Dual Coil, Active Fixation 0157/0158/0159/0164/0165/0167/ 0184/0185/0186/0187	383,000	0	0	92	571	1	3	10
ENDOTAK RELIANCE ; Dual Coil, Passive Fixation 0147/0148/0149/0174/0175/0176/0177	109,000	1	0	20	108	0	3	0
ENDOTAK RELIANCE ; Single Coil, Active Fixation 0137/0138/0160/0161/0162/0180/0181/0182	81,000	0	0	15	81	0	1	1
ENDOTAK RELIANCE ; Single Coil, Passive Fixation 0127/0128/0170/0171/0172/0173	8,000	0	0	1	6	0	0	0

S-ICD Electrodes/Model	Worldwide Distribution	Conductor	Insulation	Crimp/Weld/Bond	Other	Labeling	Packaging	Implant Accessory
EMBLEM S-ICD Electrode 3501	96,000	0	0	0	1	0	0	0
EMBLEM/Q-TRAK S-ICD Electrode 3010, 3401	43,000	0	0	1	0	0	0	0

Pacing Leads/Model	Worldwide Distribution	Conductor	Insulation	Crimp/Weld/Bond	Other	Labeling	Packaging	Implant Accessory
INGEVITY+ Positive Fixation 7840/7841/7842	724,000	0	0	0	50	0	0	0
INGEVITY Positive Fixation 7640/7641/7642/7740/7741/7742	1,120,000	2620	0	0	3346	0	0	0
INGEVITY Atrial J Passive Fixation 7635/7636/7735/7736	133,000	0	0	0	0	0	0	0
INGEVITY Passive Fixation 7631/7632/7731/7732	139,000	1	0	1	2	0	0	0
FLEXTEND 2 Active Fixation 4095/4096/4097	185,000	0	0	11	136	1	0	0
FLEXTEND Active Fixation 4086/4087/4088	290,000	0	0	66	636	1	1	4
FINELINE II ; Passive Fixation (poly) 4452/4453/4456/4457*	560,000	1	0	3	8	6	26	0
FINELINE II EZ ; Positive Fixation (poly) 4463/4464/4465/4469/4470/4471*	839,000	0	0	6	728	1	52	3
FINELINE II Atrial J (poly) 4477/4478/4479/4480*	330,000	0	0	1	144	6	18	0
FINELINE II/THINLINE II ; Passive Fixation (silicone) 4454/4455/4458/4459*	105,000	0	0	2	2	1	1	0
FINELINE II/THINLINE II EZ ; Positive Fixation (silicone) 4466/4467/4468/4472/5573/4474*	144,000	0	0	0	233	4	6	0

\*Counts consist of Boston Scientific and Intermedics co-branded pacing leads data.

Product Advisories

A Product Advisory is a voluntary letter issued to inform physicians of an anomalous device behavior identified by Boston Scientific's Quality System. A Product Advisory is issued when there is a material elevation in risk to patient safety with potential for compromised lifesaving therapy, or when Boston Scientific can provide meaningful guidance to improve patient outcomes or device performance. Boston Scientific considers many perspectives in the decision to issue a Product Advisory, including internal expertise and guidance from an independent Patient Safety Advisory Board (PSAB).

This report section includes summaries of Product Advisories for which significant, active U.S. device populations exist. In general, this includes advisories for which the estimated active U.S. advisory population is at least 200. Physician and patient letters, as well as Advisory Updates, are available at [www.bostonscientific.com](http://www.bostonscientific.com). With respect to the number of reported events listed in the summaries below, Boston Scientific recognizes that the actual number of clinical malfunctions may be greater than the number reported. Information reported in the Current Status section of each summary represents Boston Scientific's most current understanding of the data presented, but is not necessarily updated in every report. Rates and counts reported in this section may differ from those in other sections of the report due to population, geographical, methodological, or timing differences. Additionally, rate projections are provided with the acknowledgment that predictive modeling is inherently uncertain due to its dependence on the device age distribution of reported events and resultant statistical approximations and assumptions. Advisory notifications may vary by geography, based upon local regulatory requirements. Please contact the local Boston Scientific office for more information. Not all products may be approved for use in all geographies, as product approval is geography specific.

PRODUCT	ORIGINAL COMMUNICATION Jun 2021 – High Battery Impedance Initiating Safety Mode in INGENIO EL Pacemakers and CRT-Ps
Identifiable by serial number. Not all serial numbers are affected.	Voluntary Physician Advisory FDA Classification: June 2021 - Class I; Advisory update issued in Nov 2023
A serialized search tool to determine if a specific device is affected by this product advisory is available here: <a href="#">Device Lookup Tool</a>	Affected devices built with the extended life (EL) battery have the potential to transition to Safety Mode during periods of high-power consumption (e.g., interrogation by a programmer). If the battery voltage drops below a minimum threshold during a high-power state, a system reset is automatically performed, and the conditions of the high-power state are interrupted. Subsequent high-power states may result in additional system resets due to the high battery impedance. If three (3) system resets occur within a 48-hour period, the device is designed to enter Safety Mode to maintain back-up pacing with pre-defined non-programmable settings.
<b>INLIVEN CRT-P</b> Models: V284, V285, W274, W275	When a device is in Safety Mode, users are directed to contact Boston Scientific via a programmer warning screen and LATITUDE alert. Once a device enters Safety Mode, life-sustaining therapy continues to be available while battery capacity is available. The susceptibility of experiencing a high battery impedance and entering Safety Mode is increased when an affected device reaches approximately three (CRT-P) or four (DR EL) years of remaining battery longevity.
<b>INTUA CRT-P</b> Models: V272, V273, W273	
<b>INVIVE CRT-P</b> Models: V172, V173, V182, V183, W172, W173	Safety Mode provides back-up pacing under critical circumstances; it is not intended to be a substitute for chronic pacing therapy. The non-programmable Safety Mode pacing parameters may not provide optimal support of a patient's cardiac condition (e.g., adequacy of underlying escape rhythm, the need for AV/VV pacing for cardiac synchrony, and/or the potential for pacing inhibition due to myopotential oversensing).
<b>VITALIO DR EL Pacemaker</b> Models: J274, J277, K274, K277, K284	The most common clinical outcome has been early device replacement. In certain patients, Safety Mode may result in unintended clinical impact such as pacing inhibition/pauses, muscle stimulation (e.g., skeletal muscle or phrenic nerve stimulation), or heart failure prior to device replacement. The worst-case reported patient harm has been loss of pacing with serious injury or life-threatening outcome. No affected devices remain available for implant.
<b>INGENIO DR EL Pacemaker</b> Models: J174, J177, K174, K184, K187	Estimated Rate It is estimated that one third or more of affected devices will experience Safety Mode prior to reaching Explant battery indicator. The potential for life-threatening harm due to loss of pacing (occurring because of prolonged inhibition) over a device's lifetime is estimated to be less than 1 in 15,000.
<b>ADVANTIO DR EL Pacemaker</b> Models: J064, J067, K064, K084, K087	<u>November 2023 update:</u>  Since June 2021, the affected device population has aged, and additional post-market surveillance data has been collected.  Most Safety Mode reports continue to be associated with telemetry operations involving an external device. However, approximately 3.5% of reports are unrelated to telemetry operations with an external device and may occur in an ambulatory setting by transient voltage drops during normal, higher power device operations such as automatic radio frequency telemetry circuit enablement and automatic memory checks.  There have been 15 reports of a pause in pacing for older devices with less battery capacity experiencing extended transitions into Safety Mode (up to approximately 20 seconds) during telemetry operations with an external device. Thirteen (13) were associated with in-person programmer/Consult interrogations, and two (2) were associated with a LATITUDE patient initiated interrogation (PII).  When Safety Mode is initiated due to this behavior, previously reported battery time remaining estimates are invalid because they were determined without accounting for Safety Mode's increased outputs or the battery's high impedance state.  There have been three (3) deaths in pacemaker-dependent patients associated with this behavior; all were within the recommended replacement interval. Estimated Rate  The occurrence rate for this behavior is up to 8% at 9 years, 12% at 10 years, and 49% at 11 years.  The potential for life-threatening harm for the affected population is 1 in 769 (0.13%) at 11 years, which may be mitigated if devices are replaced per the recommendations below.  Standard Warranty program available, please contact your local representative for terms and conditions.
<a href="#">Safety Mode, Physician Letter, June 2021</a>	
<a href="#">Safety Mode, Patient Letter, June 2021</a>	
<a href="#">Safety Mode, Physician Letter, December 2023 Update</a>	
<a href="#">Safety Mode, Patient Letter, December 2023 Update</a>	

CURRENT STATUS 02-Jul-24

Estimated Rate of Occurrence - as of 11/2023

The occurrence rate for this behavior is up to 8% at 9 years, 12% at 10 years, and 49% at 11 years.

The potential for life-threatening harm for the affected population is 1 in 769 (0.13%) at 11 years, which may be mitigated if devices are replaced per the recommendations below.

CURRENT RECOMMENDATION 02-Jul-24

Identify patients who are at risk of harm due to Safety Mode's non-programmable parameters.

If a device enters Safety Mode, perform emergent replacement for patients who are at risk of harm. For other patients, non-emergent replacement is recommended. When choosing a replacement interval, do not rely on previously reported battery time remaining estimates which do not account for Safety Mode's increased outputs nor the battery's high impedance state.

General prophylactic replacement is not recommended. For patients who are at risk of harm, device replacement is recommended as follows:

- For DR EL pacemakers, schedule replacement when the longevity remaining is 4 years or less.
- For CRT-Ps, schedule replacement when the longevity remaining is 3 years or less.

Note: There is a potential for pacing pauses during in-person checks and LATITUDE PII in patients at risk of harm who remain implanted beyond the recommended replacement interval. During in-person device checks, consider patient recumbency and availability of resuscitation equipment with qualified personnel. Consider disabling PII for patients on LATITUDE.

Follow-up interval. Per instructions for use, perform a system follow-up via remote or in-office interrogation at least every 12 months. When longevity reaches One-Year-Remaining and then follow-up every three (3) months thereafter until replacement is indicated.

For each patient with an affected device, append their medical record with this letter to maintain awareness of this topic for the remaining service life of the device.

PRODUCT	ORIGINAL COMMUNICATION    Sep 2018 and Jun 2021 – Hydrogen-Induced Premature Depletion
Identifiable by serial number. Not all serial numbers are affected.	Voluntary Physician Advisory FDA Classification: Sep 2018 – Class II; Jun 2021 - Class II
A serialized search tool to determine if a specific device is affected by this product advisory is available here: <a href="#">Device Lookup Tool</a>	This advisory discusses two separate, distinct subsets of pacemakers and cardiac resynchronization therapy pacemakers (CRT-PS) with a potential for early pacemaker replacement due to hydrogen-induced accelerated battery depletion. The 2018 advisory population included approximately 2,900 active pacemakers, and the 2021 advisory population included approximately 125,000 active pacemakers.
<b>VALITUDE CRT-P</b> Models U125, U128	Latent release of small amounts of hydrogen within the pacemaker may compromise electrical function of a low voltage capacitor over time, resulting in accelerated depletion of the battery. The susceptibility of a pacemaker to this hydrogen-induced accelerated battery depletion mechanism is dependent upon the amount of hydrogen accumulation within the device and the susceptibility of the low voltage capacitors to hydrogen. The 2018 population is composed of pacemakers built with specific batches/lots of a liner component exhibiting a higher likelihood for this behavior. The 2021 population is composed of pacemakers built with a discontinued/original low voltage capacitor that is susceptible to compromised electrical performance in the presence of hydrogen. The use of the original low voltage capacitor in pacemaker and production of pacemakers from these advisory populations ceased in Nov 2017, and therefore they are no longer available for implantation. The most common clinical outcome has been device replacement. There have been no reported deaths associated with this behavior.
<b>VISIONIST CRT-P</b> Models U225, U226, U228	
<b>ACCOLADE Pacemaker</b> Models L300, L301, L310, L311, L321, L331	
<b>PROPONENT Pacemaker</b> Models L200, L201, L209, L210, L211, L221, L231	<i>Estimated Rate of Occurrence</i> In June 2021 Boston Scientific identified an additional population of devices and the rate of occurrence at that time is described for each population below. <ul style="list-style-type: none"> <li>The 2018 advisory subset was composed of approximately 2,100 active pacemakers. The observed malfunction rate for this behavior was 11.0% at 5 years with a potential for life-threatening harm of 1 in 500,000 (0.0002%) at 5 years.</li> <li>The 2021 advisory subset was composed of approximately 125,000 active pacemakers. The observed malfunction rate for this behavior was 1.3% at 5 years with a potential for life-threatening harm of 1 in 5,000,000 (0.00002%) at 5 years.</li> </ul>
<b>ESSENTIO Pacemaker</b> Models L100, L101, L110, L111, L121,	
<b>ALTRUA 2 Pacemaker</b> Models S701, S702, S722	Standard Warranty program available, please contact your local representative for terms and conditions.
<a href="#">Hydrogen Induced Premature Depletion, Physician Letter, September 2018</a>	<b>CURRENT STATUS    02-Jul-24</b>
<a href="#">Hydrogen Induced Premature Depletion, Patient Letter, September 2018</a>	<i>Estimated Rate of Occurrence - as of 06/2023</i> The combined 2018 and 2021 advisories subset is composed of approximately 100,000 active pacemakers. The observed malfunction rate for this behavior is 2.2% at 5 years, and 4.0% at 8 years. The observed potential for life-threatening harm is 1 in 1,000,000 (0.0001%) at 5 years.
<a href="#">Hydrogen Induced Premature Depletion, Physician Letter, June 2021</a>	More than 98% of hydrogen-induced confirmed events have been replaced before the battery reached a depleted state; therefore, normal battery assessment during labeled 12-month follow-ups is effective and recommended for both advisory populations.
<a href="#">Hydrogen Induced Premature Depletion, Patient Letter, June 2021</a>	A polymer material, designed to remove excess hydrogen within the pulse generator, was added to this device family in March 2018 and is intended to mitigate hydrogen-induced accelerated battery depletion due to the low voltage capacitors. Additionally, improvements were implemented in the liner component starting in May 2021 intended to further reduce the device's overall capacity to generate hydrogen.
	<b>CURRENT RECOMMENDATION    02-Jul-24</b> <ul style="list-style-type: none"> <li>Per labeling, perform a system follow-up via remote or in-office interrogation every 12 months until One-Year-Remaining and then every three (3) months thereafter until replacement is indicated.</li> <li>Promptly investigate any suspected indication of accelerated battery depletion, and contact Boston Scientific Technical Services for assistance as needed.</li> <li>Replace any affected pacemakers suspected of exhibiting accelerated battery depletion within 90 days of the Explant battery status indicator. Alternatively, Boston Scientific Technical Services can provide a recommended replacement interval specific to an individual device by using data from the programmer or LATITUDE. Prophylactic replacement is not recommended for pacemakers with normal battery consumption as the risk of surgical replacement outweighs the risk of accelerated battery depletion.</li> <li>For each patient with an affected device, append their medical record with this letter to maintain awareness of this topic for the remaining service life of the device.</li> </ul>

PRODUCT	<b>ORIGINAL COMMUNICATION   Dec 2020 — Model 3501 Electrode Fracture</b>
A serialized search tool to determine if a specific device is affected by this product advisory is available here: <a href="#">Device Lookup Tool</a>  <b>EMBLEM Subcutaneous Electrode</b> Model 3501  <a href="#">Model 3501 Electrode Fracture, Physician Letter, December 2020</a>  <a href="#">Model 3501 Electrode Fracture, Patient Letter, December 2020</a>	<p>Voluntary Physician Advisory FDA Classification: Class I</p> <p>This advisory discusses the performance of approximately 47,000 EMBLEM S-ICD Subcutaneous Electrodes (Model 3501). During assembly of the EMBLEM S-ICD Subcutaneous Electrode, a small amount of adhesive is applied to a location just distal to the proximal sense ring. Over time, mechanical stresses on the electrode body at this location may create the potential for a fatigue crack to initiate from the outer lumen. This crack then propagates inward toward the center-oriented distal sense conductor, eventually resulting in a fracture of the two high voltage conductors.</p> <p>The cumulative occurrence rate for this specific electrode body fracture location is 0.2% at 41 months with a potential for life-threatening harm of 1 in 25,000 (0.004%) at 10 years.</p> <p>The physician letter (link provided) details device programming considerations and troubleshooting and detection techniques.</p> <p>Standard Warranty program available, please contact your local representative for terms and conditions.</p> <p><b>CURRENT STATUS   02-Jul-24</b></p> <p><i>Estimated Rate of Occurrence - as of 03/2024</i></p> <p>The occurrence rate for EMBLEM S-ICD Subcutaneous Electrode (Model 3501) body fractures at a location just distal to the proximal sense ring is 0.32% at 81 months and the potential for life-threatening harm is 1 in 34,000 (0.0029%) at 10 years. This rate was derived by including all reports of this failure mode, whether or not the product was returned.</p> <p>An enhanced version of the EMBLEM Electrode has been developed to address the risks associated with this device behavior. Based on accelerated, extreme laboratory test, the enhanced EMBLEM Electrode design has demonstrated statistical survival of the electrode body around the sense ring to 10 implant years. Contact your local Boston Scientific sales professionals for availability.</p> <p><b>CURRENT RECOMMENDATION   02-Jul-24</b></p> <ol style="list-style-type: none"><li>1. Remote monitoring. Enroll and monitor patients through LATITUDE remote monitoring to facilitate detection of high electrode impedance alert or non-physiologic, mechanical artifacts on stored S-ECGs during the interval between in-office device checks. Instruct patients to comply with weekly remote interrogations.</li><li>2. Follow-up interval. Perform a system follow-up every three months via remote or in-office interrogation.</li><li>3. During follow-ups. For every remote or in-office follow-up:<ol style="list-style-type: none"><li>3.1. Promptly investigate any high impedance alerts in-clinic, as this may indicate an electrode body fracture and an inability of the system to provide therapy.</li><li>3.2. Review stored episode S-ECGs for non-physiologic, mechanical artifacts, as this may indicate onset of electrode body fracture.</li><li>3.3. During in-clinic follow-up, capture all sensing vectors, and review for the following conditions, any of which may indicate onset of electrode body fracture:<ol style="list-style-type: none"><li>3.3.1. cardiac signals on the S-ECGs of the Primary and Secondary sensing vector look nearly identical; or</li><li>3.3.2. flatline S-ECGs in the Alternate sensing vector.</li></ol></li><li>3.4. Assess sensing performance in-clinic during isometrics and/or posture changes if any of the following is observed: non-physiologic, mechanical artifacts and/or high electrode impedance alerts. If isometrics and/or posture changes provoke non-physiologic, mechanical artifacts, this may indicate onset of an electrode body fracture.</li></ol></li><li>4. Imaging. If an electrode body fracture is suspected, perform chest radiography in PA and left lateral view projections, ensuring the entire electrode length can be visualized to enable differential diagnosis of competing causes of high impedance or artifact signals. Portable X-ray images typically provide insufficient clarity to evaluate electrode integrity. In the absence of any indications of electrode fracture, surveillance X-rays are not recommended.</li><li>5. Shocks and beeping tones. During the next in-office follow-up visit, demonstrate the device beeper to the patient using the programmer's Test Beeper function available from the Beeper Control screen within the Utilities menu.<ul style="list-style-type: none"><li>- For patients not monitored by LATITUDE, repeat the beeper demonstration following any MRI scan, as strong magnetic fields may cause permanent loss of beeper volume; and</li><li>- Remind all patients to promptly contact their physician if beeping tones are heard from their device or if a shock is delivered.</li></ul></li><li>6. Evaluate risk. The potential for life-threatening harm due to an electrode body fracture is greatest for:<ul style="list-style-type: none"><li>- patients with a history of life-threatening ventricular arrhythmias such as secondary prevention indication or previous appropriate shock for VT/VF;</li><li>- patients who are unable to be reliably followed remotely or in person every three months; or</li><li>- patients who are not monitored via LATITUDE and are unable to hear beeping tones</li></ul></li><li>7. Replacement. Following consultation with Boston Scientific Technical Services, promptly replace any electrode that is indicated to have compromised integrity as evidenced by non-physiologic, mechanical artifacts, high impedance alert, and/or X-ray. Routine prophylactic replacement of an electrode without evidence of fracture is not recommended. Return explanted devices to Boston Scientific.</li><li>8. De novo and replacement S-ICD candidates. Consider overall S-ICD performance with respect to the competing risks for transvenous ICDs. The Product Performance Report includes up-to-date performance data on Boston Scientific transvenous leads and subcutaneous electrodes.</li></ol>

PRODUCT	ORIGINAL COMMUNICATION Dec 2020 — EMBLEM S-ICD Electrical Overstress
Identifiable by serial number. Not all serial numbers are affected.	Voluntary Physician Advisory FDA Classification: Class I
A serialized search tool to determine if a specific device is affected by this product advisory is available here: <a href="#">Device Lookup Tool</a>	This advisory discusses the potential for a specific subset of approximately 3,350 EMBLEM™ Subcutaneous Implantable Cardioverter Defibrillators (S-ICDs) (Model A209 and A219) to experience a malfunction during high voltage therapy delivery, necessitating device replacement due to electrical overstress (i.e., damage to the device caused by electrical shorting).
<b>EMBLEM S-ICD</b> Models A209, A219	Laboratory analysis of the returned devices confirmed evidence of electrical overstress damage in the device feedthrough area. Investigation has shown that, over time, variations in header assembly allowed a very small pathway for moisture ingress enabling a shorting condition to occur during delivery of high voltage therapy. Each of the devices exhibiting electrical overstress were built within a specific timeframe (between May 2015 through December 2017); a header assembly subprocess was found to be subject to process variations directly contributing to this behavior. There is no available method to detect whether an individual device is vulnerable to this condition prior to its occurrence. It is important to note that not all S-ICDs built during this timeframe were exposed to these process variations.
<a href="#">EMBLEM Electrical Overstress, Physician Letter, December 2020</a>	<i>Estimated Rate of Occurrence</i> <ul style="list-style-type: none"><li>• Boston Scientific has confirmed six (6) events of EMBLEM S-ICD electrical overstress malfunctions that have occurred in association with delivery of high voltage therapy. These events manifested clinically by the subsequent inability to interrogate the device or by display of device-based errors/alerts. Boston Scientific Technical Services recommended device replacement in each instance, and no serious patient injury or death has been reported.</li><li>• The projected occurrence rate for this electrical overstress behavior is 0.3% at 5 years, and the most common clinical outcome is early device replacement. Although there have been no serious injuries reported to date, the potential exists for life-threatening harm due to an inability to provide needed defibrillation therapy, as it is possible that either all or a portion of programmed defibrillation shock energy may not actually be delivered in the event of an electrical overstress malfunction. We estimate that the probability of the hypothetical worst-case harm associated with loss of ambulatory ventricular tachycardia/ventricular fibrillation therapy resulting in death is 0.09% at 5 years</li></ul>
<a href="#">EMBLEM Electrical Overstress, Patient Letter, December 2020</a>	Standard Warranty program available, please contact your local representative for terms and conditions.
	<b>CURRENT STATUS 02-Jul-24</b>
	<i>Estimated Rate of Occurrence - as of 08/2021</i> <ul style="list-style-type: none"><li>• The projected occurrence rate for this electrical overstress behavior is 0.3% at 5 years, and the most common clinical outcome is early device replacement.</li><li>• We estimate that the probability of the hypothetical worst-case harm associated with loss of ambulatory ventricular tachycardia/ventricular fibrillation therapy resulting in death is 0.09% at 5 years</li></ul>
	<b>CURRENT RECOMMENDATION 02-Jul-24</b>
	1. Remote monitoring. Enroll and monitor patients through the LATITUDE NXT Patient Management System to facilitate prompt detection of accelerated depletion or alert conditions such as ERI or EOL during the interval between in-office device checks. Instruct patients to comply with remote checks and interrogations. 2. Follow-up interval. Perform a system follow-up every 3 months per labeling via remote or in-office interrogation. 3. During follow-ups. Promptly investigate any suspected indication of accelerated battery depletion, and contact Boston Scientific Technical Services for assistance as needed. 4. Demonstrate beeping tones. During the next in-office follow-up visit, demonstrate the device beeper to the patient using the programmer's Test Beeper function available from the Beeper Control screen within the Utilities menu. - For patients not monitored by LATITUDE, repeat the beeper demonstration following any MRI scan as strong magnetic fields may cause permanent loss of beeper volume; and - Remind patients to promptly contact their physician if beeping tones are heard from their device as this may be an indication of ERI. 5. Evaluate risk. The potential for life-threatening harm due to accelerated depletion is greatest for: - Patients with a history of life-threatening ventricular arrhythmias such as secondary prevention indication or previous appropriate shock for ventricular arrhythmias; - Patients who are unable to be reliably followed remotely or in person every 3 months; or - Patients who are not monitored via LATITUDE and are unable to hear beeping tones. 6. Replacement. Replace any affected EMBLEM S-ICD suspected of exhibiting accelerated battery depletion within 21 days of ERI. Alternatively, Boston Scientific Technical Services can provide a recommended replacement interval specific to an individual device by using data from the programmer or LATITUDE. - In other cases of high risk, as indicated by the factors listed above, consider prophylactic device replacement after taking individual patient preferences and circumstances into account through a process of shared decision-making. - Return explanted devices to Boston Scientific. A no cost Return Product kit is available from your local Boston Scientific representative.

PRODUCT	ORIGINAL COMMUNICATION Aug 2019 and Dec 2020 — EMBLEM S-ICD Premature Depletion
Identifiable by serial number. Not all serial numbers are affected.	Voluntary Physician Advisory FDA Classification August 2019: Class II
A serialized search tool to determine if a specific device is affected by this product advisory is available here: <a href="#">Device Lookup Tool</a>	FDA Classification December 2020: Class II  In August 2019, a physician communication discussed a subset of EMBLEM™ Subcutaneous Implantable Cardioverter Defibrillators (S-ICDs) that may result in a need for device replacement (ERI/EOL) earlier than expected due to compromised performance of an electrical component causing accelerated battery depletion.
<b>EMBLEM S-ICD</b> Models A209, A219	In December 2020, the advisory population was expanded to a total of approximately 42,000 distributed EMBLEM S-ICDs with an elevated likelihood of a low voltage capacitor causing accelerated battery depletion. This behavior can be detected if an unexpected decrease in remaining battery capacity is observed between remote/in-clinic follow-ups. Progression of accelerated depletion eventually produces a battery status replacement indicator (ERI) which is detectable through ambulatory beeping tones, remote monitoring, or in-clinic follow-up. Devices exhibiting this accelerated depletion behavior are capable of providing therapy for a minimum of 21 days after ERI independent of when EOL is initiated.
<a href="#">EMBLEM Premature Depletion, Physician Letter, August 2019</a>	The most common clinical outcome associated with this device behavior is early replacement. In August 2018, Boston Scientific transitioned S-ICDs to an alternative low voltage capacitor. All EMBLEM S-ICDs with the original low voltage capacitor are included in either the original or the expanded advisory population and none are available for implantation.
<a href="#">EMBLEM Premature Depletion, Patient Letter, August 2019</a>	<i>Estimated Rate of Occurrence</i> • The August 2019 advisory subset is comprised of approximately 400 distributed worldwide devices manufactured in July 2017. The August 2019 advisory subset has a projected rate of accelerated depletion of 15.1% at 5 years with a projected potential for life-threatening harm in this subset of approximately 1 in 50,000 at 5 years.
<a href="#">EMBLEM Premature Battery Depletion Physician Letter Update, December 2020</a>	• The December 2020 advisory subset is comprised of approximately 42,000 distributed worldwide devices manufactured before August 2018. The December 2020 advisory subset has a projected rate of accelerated depletion of 3.7% at 5 years with a projected potential for life-threatening harm in this subset of approximately 1 in 250,000 at 5 years.
<a href="#">EMBLEM Premature Battery Depletion Physician Letter Update, February 2022</a>	
<a href="#">EMBLEM Premature Depletion, Patient Letter Update, February 2022</a>	Standard Warranty program available, please contact your local representative for terms and conditions.
	<b>CURRENT STATUS 02-Jul-24</b>
	The existing Battery Depletion (BD) alert has been enhanced to enable detection of hydrogen-induced accelerated battery depletion in Model A209 and A219 EMBLEM S-ICDs. Affected devices must be interrogated by a programmer with updated software.
	<i>Estimated Rate of Occurrence - as of 07/2024</i> Because the 5-year malfunction rate for the August 2019 and December 2020 populations has converged, a single malfunction rate is reported for the combined populations. There are approximately 17,000 active worldwide devices.  The malfunction rate is 10.2% at 5 years, 23.1% at 6 years, and 33.1% at 7 years. The projected potential for life-threatening harm is approximately 1 in 110,000 at 5 years.

CURRENT RECOMMENDATION 02-Jul-24

Recommendations for countries where enhanced BD alert software upgrade is available. Contact your local Boston Scientific sales representative to determine availability of software in your country.

- 1. Programmer Software Upgrade. Confirm programmers at your center have been upgraded.
  - Model 3300 LATITUDE Programmers are supported with Model 3877 v1.03 application
  - Model 3200 EMBLEM Programmers are supported with Model 2877 v4.09 application
- 2. Next Follow-up. Boston Scientific continues to recommend 3-month follow-ups per labeling. Bearing in mind the risk versus benefits of in-person visits in the setting of the global COVID-19 pandemic, consider an in-person visit at the next scheduled follow-up, so the enhanced BD alert can be enabled in each affected device.
  - When an EMBLEM S-ICD is first interrogated by an upgraded programmer, an S-ICD software update will be performed. Per labeling, monitor the patient and have external defibrillation equipment available as tachycardia therapy is suspended during a S-ICD software update.
  - If a BD alert occurs, follow screen prompts and contact Technical Services. Using device data, Technical Services can provide a replacement interval.
- 3. Update Records. For each patient with an affected EMBLEM S-ICD, append their medical record with this letter to maintain awareness of this topic for the remaining service life of the device.

Follow-up Recommendations:

- 1. Remote monitoring. Enroll and monitor patients through the LATITUDE NXT Patient Management System to facilitate prompt detection of accelerated depletion or alert conditions such as ERI or EOL during the interval between in-office device checks. Instruct patients to comply with remote checks and interrogations.
- 2. Follow-up interval. Perform a system follow-up every 3 months per labeling via remote or in-office interrogation.
- 3. During follow-ups. Promptly investigate any suspected indication of accelerated battery depletion, and contact Boston Scientific Technical Services for assistance as needed.
- 4. Demonstrate beeping tones. During the next in-office follow-up visit, demonstrate the device beeper to the patient using the programmer's Test Beeper function available from the Beeper Control screen within the Utilities menu.
  - For patients not monitored by LATITUDE, repeat the beeper demonstration following any MRI scan as strong magnetic fields may cause permanent loss of beeper volume; and
  - Remind patients to promptly contact their physician if beeping tones are heard from their device as this may be an indication of ERI.
- 5. Evaluate risk. The potential for life-threatening harm due to accelerated depletion is greatest for:
  - Patients with a history of life-threatening ventricular arrhythmias such as secondary prevention indication or previous appropriate shock for ventricular arrhythmias;
  - Patients who are unable to be reliably followed remotely or in person every 3 months; or
  - Patients who are not monitored via LATITUDE and are unable to hear beeping tones.
- 6. Replacement. Replace any affected EMBLEM S-ICD suspected of exhibiting accelerated battery depletion within 21 days of ERI. Alternatively, Boston Scientific Technical Services can provide a recommended replacement interval specific to an individual device by using data from the programmer or LATITUDE.
  - In other cases of high risk, as indicated by the factors listed above, consider prophylactic device replacement after taking individual patient preferences and circumstances into account through a process of shared decision-making.
  - Return explanted devices to Boston Scientific. A no cost Return Product kit is available from your local Boston Scientific representative.

PRODUCT	ORIGINAL COMMUNICATION November 2018 — SQ-RX 1010 Shortened Replacement Time
Identifiable by serial number. Not all serial numbers are affected.	Voluntary Physician Advisory FDA Classification: Unclassified
A serialized search tool to determine if a specific device is affected by this product advisory is available here: <a href="#">Device Lookup Tool</a>	This advisory discusses the potential for a shortened replacement interval after a Charge Time (CT) / Battery Depletion (BD) alert has occurred or after the battery status reaches Elective Replacement Indicator (ERI) in the first-generation Subcutaneous Implantable Cardioverter Defibrillator (S-ICD) system's SQ-RX™ Model 1010 Pulse Generator (PG).
<b>S-ICD</b> Model 1010	The SQ-RX Model 1010 PG provides an Elective Replacement Indicator (ERI) as the PG approaches the end of its expected battery service life. When the battery reaches ERI through normal use, there is sufficient capacity to support up to 90 days of continued operation, including up to 6 maximum energy charges/shocks before fully depleting. However, if the PG experiences a latent battery malfunction resulting in accelerated battery depletion, the reserve battery capacity available beyond ERI may not be sufficient to support the full 90-day interval or additional shock therapy before depleting. The rate of depletion for a latent battery malfunctions varies.
<a href="#">SQ-RX 1010 Shortened Replacement Time, Physician Letter, November 2018</a>	The SQ-RX model 1010 PGs include separate monitors for charging and battery performance. The Charge Time (CT) alert is designed to detect unsuccessful charging of the high voltage capacitors within 44 seconds. The Battery Depletion (BD) alert is designed to detect higher rates of accelerated battery depletion. When an alert condition occurs, the patient is notified through beeping tones and the clinician user is notified through programmer messages. Most battery malfunctions exhibit a sufficient rate of accelerated depletion to be detected by one of these alerts. Some battery malfunctions exhibit a slower rate of accelerated depletion, which is not detected as an alert condition. Based on an analysis of accelerated battery depletion events where only ERI presented (no alert condition), at least one maximum energy shock has been determined to be available for at least 20 days after ERI.
<a href="#">SQ-RX 1010 Shortened Replacement Time, Patient Letter, November 2018</a>	<i>Estimated Rate of Occurrence</i> The projected occurrence rate for latent battery malfunctions for SQ-RX Model 1010 PGs is up to 2% at 5 years. There have been no reports of injuries or deaths associated with this behavior. Laboratory analysis of returned PGs with latent battery malfunctions has shown some depletions to a level at which therapy would not have been available if not replaced in accordance with the recommendations above. Based on a 3-month follow-up interval, the potential for life threatening harm for this behavior is 0.006% (1 in 16,667) at 5 years. However, the potential for life-threatening harm is greater for secondary prevention patients or those who have received appropriate therapy previously, patients with longer follow-up intervals, and/or patients who are unable to hear beeping tones. For these patients, the benefit associated with prophylactically replacing the PG may outweigh the risks associated with a shortened replacement interval due to latent battery malfunction.  Standard Warranty program available, please contact your local representative for terms and conditions.
	<b>CURRENT STATUS 02-Jul-24</b>
	<i>Estimated Rate of Occurrence - as of 10/2018</i> The projected occurrence rate for latent battery malfunctions for SQ-RX Model 1010 PGs is up to 2% at 5 years.
	<b>CURRENT RECOMMENDATION 02-Jul-24</b>
	<ul style="list-style-type: none"><li>• <u>Follow-Up.</u> Consistent with the SQ-RX Model 1010 PG User Manual:<ul style="list-style-type: none"><li>- Perform in-clinic checks every 3 months as the PG is not capable of remote patient management;</li><li>- If it has been more than 3 months since a patient's last in-clinic follow-up, schedule a follow-up within the next month and every 3 months thereafter;</li><li>- During the next follow-up visit, demonstrate the beeper by applying a magnet over the PG to elicit beeping tones; and</li><li>- Remind patients to promptly contact their physician if beeping tones are heard from their PG as this may be an indication of a CT / BD alert or ERI.</li><li>- Append the patient's medical record with this letter to maintain awareness of this topic for the remaining service life of their PG</li></ul></li><li>• <u>Evaluate Risk.</u> The potential for life-threatening harm is greater for patients who have experienced life-threatening ventricular arrhythmias, patients not followed every 3 months, and/or patients who are unable to hear beeping tones. For these patients, the benefit associated with prophylactically replacing the PG may outweigh the risks associated with a shortened replacement interval due to latent battery malfunction</li><li>• <u>CT / BD Alerts.</u> Promptly investigate any beeping tones, CT alerts, or BD alerts and report them to Boston Scientific Technical Services. Using saved PG data, Technical Services can determine if an accelerated battery depletion exists and provide guidance for replacement.</li><li>• <u>ERI.</u> To mitigate the rare potential for undetected accelerated battery depletion, replace SQ-RX Model 1010 PGs within 20 days of ERI. If a longer replacement interval is desired, save PG data and contact Technical Service to determine a recommended replacement interval. Note: CT / BD Alerts appearing before or after ERI should always be reported to Technical Services for evaluation</li></ul>

PRODUCT	ORIGINAL COMMUNICATION    December 2017 — Minute Ventilation Signal Oversensing												
A serialized search tool to determine if a specific device is affected by this product advisory is available here: <a href="#">Device Lookup Tool</a>	Voluntary Physician Advisory												
<b>VALITUDE CRT-P</b> Models U125, U128	This advisory discusses intermittent oversensing of the Minute Ventilation (MV) sensor signal with certain Boston Scientific pacemaker and cardiac resynchronization therapy pacemaker systems (pacemakers). MV sensor signal oversensing may cause pre-syncope or syncope due to periods of pacing inhibition. This MV behavior may occur with any manufacturer's pacing lead system, but Boston Scientific has determined it to be more likely for affected Boston Scientific pacemakers using Medtronic or Abbott/St. Jude (Abbott) leads implanted in either the right atrium (RA) or right ventricle (RV).												
<b>VISIONIST CRT-P</b> Models U225, U226, U228	The MV sensor in Boston Scientific pacemakers can be used for RightRate™ (rate adaptive pacing), Respiratory Rate Trend, or AP Scan. When the RA/RV pacing leads and lead terminal connections are operating as intended, the MV sensor signal is appropriately filtered and therefore is not detected by the pacemaker or displayed on electrograms (EGMs). However, intermittency related to the lead or pacemaker-lead connection has the potential to create a transient high impedance condition. A high impedance condition may subsequently alter the MV sensor signal such that it becomes visible on EGMs and potentially subject to oversensing on the RA or RV channels. For a technical description of the Boston Scientific's MV sensor, please refer to Appendix A in the December 2017 physician letter.												
<b>ACCOLADE Pacemaker</b> Models L300, L301, L310, L311, L321, L331	Engineering analysis and testing, as well as evaluation of post-market surveillance data, demonstrates an elevated potential for oversensing of the MV sensor signal in certain pacemaker systems connected to Medtronic or Abbott pacing leads. Although all leads evaluated in simulated testing environments comply with appropriate connector standards, we have discovered subtle differences amongst lead manufacturers in the surface finish of the lead terminal ring and amount of axial and radial terminal ring motion within the pacemaker header. These factors may result in intermittent increases in impedance leading to oversensing of the MV sensor signal or changes in daily impedance test measurements.												
<b>PROPONENT Pacemaker</b> Models L200, L201, L209, L210, L211, L221, L231													
<b>ESSENTIO Pacemaker</b> L131													
<b>ALTRUA 2 Pacemaker</b> Models S701, S702, S722	<i>Estimated Rate of Occurrence</i>  Boston Scientific investigation has shown that the probability of harm associated with MV sensor signal oversensing behavior is significantly greater when affected pacemakers are connected to Medtronic or Abbott pacing leads.												
<a href="#">Minute Ventialtion Signal Oversensing, Physician Letter, December 2017</a>	<table><tr><th>Affected pacemaker systems connected to the following RA/RV pacing leads:</th><th>Probability of Injury at 5 years</th><th>Probability of Life Threatening Harm at 5 years</th></tr><tr><td>Medtronic or Abbott pacing leads</td><td>0.0005 (1 in 2,000)</td><td>0.00001 (1 in 100,000)</td></tr><tr><td>Boston Scientific pacing leads (including DEXTRUS)</td><td>0.00003 (1 in 33,333)</td><td>0.0000008 (1 in 1,250,000)</td></tr><tr><td>All pacing leads combined</td><td>0.00008 (1 in 12,500)</td><td>0.000002 (1 in 500,000)</td></tr></table>	Affected pacemaker systems connected to the following RA/RV pacing leads:	Probability of Injury at 5 years	Probability of Life Threatening Harm at 5 years	Medtronic or Abbott pacing leads	0.0005 (1 in 2,000)	0.00001 (1 in 100,000)	Boston Scientific pacing leads (including DEXTRUS)	0.00003 (1 in 33,333)	0.0000008 (1 in 1,250,000)	All pacing leads combined	0.00008 (1 in 12,500)	0.000002 (1 in 500,000)
Affected pacemaker systems connected to the following RA/RV pacing leads:	Probability of Injury at 5 years	Probability of Life Threatening Harm at 5 years											
Medtronic or Abbott pacing leads	0.0005 (1 in 2,000)	0.00001 (1 in 100,000)											
Boston Scientific pacing leads (including DEXTRUS)	0.00003 (1 in 33,333)	0.0000008 (1 in 1,250,000)											
All pacing leads combined	0.00008 (1 in 12,500)	0.000002 (1 in 500,000)											
<a href="#">Minute Ventialtion Signal Oversensing, Patient Letter, December 2017</a>	<b>CURRENT STATUS    02-Jul-24</b>												
<a href="#">Minute Ventialtion Signal Oversensing, Update letter, January 2019</a>	Software has been developed that eliminates the risk of pacing inhibition due to Minute Ventilation (MV) sensor signal oversensing in pacemakers and cardiac resynchronization therapy pacemaker (CRT-P) systems. The software includes a Signal Artifact Monitor (SAM) which further expands our proprietary suite of Safety Architecture automatic self-diagnostics. Once programmers are upgraded with this software, the SAM is automatically enabled whenever the MV sensor is enabled and continuously monitors electrograms for MV sensor signal artifacts. If MV artifacts are detected, the SAM either switches to the right ventricular vector or disables the MV sensor in approximately one second thus eliminating the risk of pacing inhibition due to MV sensor signal oversensing. Contact your local Boston Scientific sales representative to find out if this software is available in your country.												
	<b>CURRENT RECOMMENDATION    02-Jul-24</b>												
	Software is available in most countries to address the potential for pacing inhibition due to MV sensor signal oversensing in affected pacemakers. The software adds the Signal Artifact Monitor (SAM) to Boston Scientific's proprietary suite of Safety Architecture diagnostics. When enabled, the SAM continuously monitors electrograms for MV sensor signal artifacts and measures MV vector lead impedance values. If artifacts are detected or the MV vector lead impedance is out of range, the monitor either switches to the right ventricular vector or disables the MV sensor in approximately one second. In this manner, the SAM promptly eliminates the clinical risk of pacing inhibition associated with MV sensor signal oversensing.												
	<table><tr><th>Programmer</th><th>Software Model</th><th>Software Version</th></tr><tr><td>Model 3120 ZOOM Programmer</td><td>2869</td><td>2.06</td></tr><tr><td>Model 3300 LATITUDE Programmer</td><td>3869</td><td>1.05</td></tr></table>	Programmer	Software Model	Software Version	Model 3120 ZOOM Programmer	2869	2.06	Model 3300 LATITUDE Programmer	3869	1.05			
Programmer	Software Model	Software Version											
Model 3120 ZOOM Programmer	2869	2.06											
Model 3300 LATITUDE Programmer	3869	1.05											
	If software is not available in your country, continue to follow advisory recommendations.												

PRODUCT	ORIGINAL COMMUNICATION December 2017 — CRT Positive LV Offset and TPP Interaction																				
Identifiable by serial number. Not all serial numbers are affected.	Voluntary Physician Advisory FDA Classification: Unclassified																				
A serialized search tool to determine if a specific device is affected by this product advisory is available here: <a href="#">Device Lookup Tool</a>	This advisory discusses unintended asynchronous biventricular (BiV) pacing behavior when tracking elevated atrial intrinsic rhythms in certain Boston Scientific Cardiac Resynchronization Therapy (CRT) pacemakers (CRT-Ps) and defibrillators (CRT-Ds). Repeated detection of this unintended asynchronous BiV pacing behavior may result in the implanted device reverting to a permanent Safety Mode (Safety Core™) status thus requiring early replacement. The unintended asynchronous BiV pacing behavior can only occur when an infrequent combination of parameters are programmed, specifically: <ul style="list-style-type: none"><li>• Left Ventricular (LV) Offset programmed to a positive value which exceeds the Atrial Blank after Ventricular Pace (A-Blank after V-Pace) interval; and</li><li>• Tracking Preference = ON (nominal).</li></ul>																				
<b>VALITUDE CRT-P</b> Models U125, U128	<i>Observed Rate</i> Of the 60,500 CRT devices distributed worldwide, Boston Scientific estimates approximately 300 CRT devices are programmed with the combination of parameters which may lead to this device behavior. There have been two confirmed instances of early device replacement due to this device behavior (0.7%). Of the two cases, a single patient death occurred due to complications related to the replacement procedure.																				
<b>VISIONIST CRT-P</b> Models U225, U226, U228																					
<b>RESONATE CRT-D</b> Models G424, G425, G426, G428, G437, G447, G448, G524, G525, G526, G528, G537, G547, G548																					
<b>VIGILANT CRT-D</b> Models G224, G225, G228, G237, G247, G248																					
<b>MOMENTUM CRT-D</b> Models G124, G125, G126, G128, G138																					
<b>CHARISMA CRT-D</b> G337, G347, G348	<b>CURRENT STATUS 02-Jul-24</b> <i>Confirmed Malfunctions (worldwide)</i> There have been five confirmed instances of early device replacement due to this device behavior.																				
<b>AUTOGEN CRT-D</b> Models G172, G173, G175, G177, G179	<b>CURRENT RECOMMENDATION 02-Jul-24</b> Software is available in most countries to addresses the rare potential for early replacement due to permanent Safety Mode status. The software imposes an interactive limit which prevents programming the device into a susceptible manner. Affected devices interrogated by an updated programmer are no longer susceptible to this issue.																				
<b>DYNAGEN CRT-D</b> Models G150, G151, G156, G158	<table><tr><th>Programmer</th><th>Device Therapy</th><th>Software Model</th><th>Software Version</th></tr><tr><td>Model 3120 ZOOM Programmer</td><td>CRT-Ps</td><td>2869</td><td>2.06</td></tr><tr><td>Model 3300 LATITUDE Programmer</td><td>CRT-Ps</td><td>3869</td><td>1.05</td></tr><tr><td>Model 3120 ZOOM Programmer</td><td>CRT-Ds</td><td>2868</td><td>4.07</td></tr><tr><td>Model 3300 LATITUDE Programmer</td><td>CRT-Ds</td><td>3868</td><td>1.07</td></tr></table>	Programmer	Device Therapy	Software Model	Software Version	Model 3120 ZOOM Programmer	CRT-Ps	2869	2.06	Model 3300 LATITUDE Programmer	CRT-Ps	3869	1.05	Model 3120 ZOOM Programmer	CRT-Ds	2868	4.07	Model 3300 LATITUDE Programmer	CRT-Ds	3868	1.07
Programmer	Device Therapy	Software Model	Software Version																		
Model 3120 ZOOM Programmer	CRT-Ps	2869	2.06																		
Model 3300 LATITUDE Programmer	CRT-Ps	3869	1.05																		
Model 3120 ZOOM Programmer	CRT-Ds	2868	4.07																		
Model 3300 LATITUDE Programmer	CRT-Ds	3868	1.07																		
<b>INOGEN CRT-D</b> Models G140, G141, G146, G148	If software is not available in your country, continue to follow advisory recommendations.																				
<b>ORIGEN CRT-D</b> Models G050, G051, G056, G058																					
<a href="#">CRT Positive LV Offset and TPP Interaction, Physician Letter, Dec 2017</a>																					
<a href="#">CRT Positive LV Offset and TPP Interaction, Patient Letter, December 2017</a>																					
<a href="#">CRT Positive LV Offset and TPP Interaction, Update Letter, January 2019</a>																					

PRODUCT	ORIGINAL COMMUNICATION Aug 2013 and Sep 2014 — Low Voltage Capacitor
<p>A serialized search tool to determine if a specific device is affected by this product advisory is available here:</p> <p><a href="#">Device Lookup Tool</a></p> <p><b>COGNIS</b> Models N106/N107/N108/N118/ N119/N120/P106/P107/P108</p> <p><b>TELIGEN VR</b> Models E102/E103/F102/F103</p> <p><b>TELIGEN DR</b> Models E110/E111/F110/F111</p> <p><a href="#">Low Voltage Capacitor 2014 Physician Letter, Sep 17, 2014</a></p> <p><a href="#">Low Voltage Capacitor 2014 Patient Letter, Sep 17, 2014</a></p> <p><a href="#">Low Voltage Capacitor 2013 Physician Letter, Aug 29, 2013</a></p>	<p>Voluntary Physician Advisory FDA Classification August 2013: Class II FDA Classification September 2014: Class II</p> <p>In August 2013, a physician communication discussed a subset of COGNIS CRT-Ds and TELIGEN ICDs that had experienced an increased rate of premature battery depletion due to compromised performance of a low voltage (LV) capacitor. It also informed physicians how to identify and respond to a Safety Architecture low voltage alert. In September 2014, a second subset of devices was identified that may exhibit compromised LV capacitor performance at a rate that is similar to the August 2013 advisory subset. The second communication also discussed improvements to Safety Architecture's low voltage alert, which were released through a programmer software update.</p> <p>The performance of an LV capacitor may be compromised in some devices after two or more years of implant time, which will increase battery use and may eventually initiate one or more Safety Architecture alerts and patient-audible beeping.</p> <p>The most common alert is a yellow programmer screen that states, “Voltage is too low for projected remaining capacity. Contact Technical Services with Code 1003”. LATITUDE issues a corresponding yellow alert (nominally configured “On”). In other instances, diminished LV capacitor performance can result in an early “Explant” battery status indicator (ERI) and a replacement window that may be less than 3 months.</p> <p>Devices that experience a low voltage alert require replacement. If not replaced, increased current drain could deplete the battery and impact therapy delivery and telemetry.</p> <p><u>Advisory population</u> Approximately 22,800 devices identified in the August 2013 communication remain in service. In September 2014, Boston Scientific identified an additional 27,300 active devices that may exhibit diminished LV capacitor performance at a rate that is similar to the August 2013 advisory population. The projected cumulative rate of occurrence for LV capacitor malfunction within the total advisory population is approximately 2.9% at 60 months. Due to Safety Architecture alerts and timely physician response, the potential for life-threatening harm from loss of therapy is estimated to be less than 1 in 125,000 (0.0008%) at 60 months.</p> <p><b>CURRENT STATUS 02-Jul-24</b></p> <p><i>Estimated Rate of Occurrence - as of 01/2022</i></p> <ul style="list-style-type: none"><li>• COGNIS CRT-D and TELIGEN ICD advisory population - The rate of occurrence is 2.8% at 60 months, 5.8% at 72 months, 8.6% at 84 months, 10.9% at 96 months, 12.2% at 108 months, and 12.9% at 120 months. The potential for life-threatening harm from loss of therapy is approximately 1 in 200,000 (0.0005%) at 60 months.</li><li>• COGNIS CRT-D and TELIGEN ICD populations (advisory and non-advisory) - The overall rate of occurrence is approximately 1.1% at 60 months, 2.4% at 72 months, 3.9% at 84 months, 5.2% at 96 months, 6.0% at 108 months, and 6.2% at 120 months . Since notifying customers of this behavior in September 2014 and improving the Safety Architecture voltage alert, the portion of malfunctions with compromised therapy is approximately 2.2%. The potential for life-threatening harm from loss of therapy is approximately 1 in 500,000 (0.0002%) at 60 months.</li><li>• INCEPTA, ENERGEN and PUNCTUA CRT-Ds and ICDs - The rate of occurrence is 1.1% at 60 months, 2.0% at 72 months, 3.0% at 84 months, 3.8% at 96 months, 4.3% at 108 months, and 4.5% at 120 months. The portion of malfunctions with compromised therapy is approximately 0.3%. The potential for life-threatening harm from loss of therapy is approximately 1 in 2,500,000 (0.00004%) at 60 months.</li></ul> <p><b>CURRENT RECOMMENDATION 02-Jul-24</b></p> <p><u>Updated Software</u> In 2014 BSC released software that enhances the effectiveness of the Safety Architecture tools later in device life. When the software was introduced, BSC recommended an in-clinic follow-up with an updated programmer at first opportunity, but within 3 months for patients within the advisory population. In-clinic interrogation with a current programmer automatically downloads Safety Architecture software upgrades from the programmer into individual patient devices, enhancing detection of a compromised LV capacitor before therapy delivery is impacted.</p> <p><u>LATITUDE Patient Management System</u> Boston Scientific recommends that advisory patients utilize the LATITUDE Patient Management System (remote monitoring), which offers additional/supplemental device checks between office visits. Use of LATITUDE may accelerate detection of Safety Architecture alerts, and can notify if/when scheduled checkups have not occurred. Verify that the yellow alert “Voltage was too low for projected remaining capacity” is configured “On”.</p> <p><u>Additional Recommendations</u></p> <ul style="list-style-type: none"><li>- After a device has been upgraded with new software, Boston Scientific recommends normal device monitoring as described in device labeling.</li><li>- Device replacement is not recommended for advisory devices displaying normal behavior.</li><li>- Promptly investigate alerts, device beeping, and unanticipated replacement indicator messages.</li><li>- Following a Safety Architecture alert, contact Boston Scientific Technical Services as directed on programmer screens. Technical Services can facilitate an evaluation of device information downloaded from a recent in-clinic or remote LATITUDE interrogation, which may help to clarify available replacement time.</li></ul> <p>Standard Warranty program available, please contact your local representative for terms and conditions.</p>

PRODUCT	ORIGINAL COMMUNICATION 01-Dec-09 — Subpectoral Implant
A serialized search tool to determine if a specific device is affected by this product advisory is available here: <a href="#">Device Lookup Tool</a>	Voluntary Physician Advisory FDA Classification: Class II
<i>This advisory is limited to those models listed below implanted subpectorally.</i>	This advisory is limited to devices identified in the product model list that were implanted subpectorally. Devices implanted subcutaneously are not included in this advisory.
<b>COGNIS</b> Models N106/N107/N108/N118/N119 P106/P107/P108	Boston Scientific has determined that the bond between the header and case could be weakened by significant forces associated with a subpectoral implant procedure or when a device in a subpectoral position is pushed against a rib during contraction of the pectoralis muscle. A weakened header bond may alter lead impedance and introduce noise that may inhibit pacing therapy or initiate inappropriate tachy therapy. Additional mechanical stress applied to a weakened bond may eventually cause header connection wires to fracture, resulting in loss of therapy.
<b>TELIGEN VR</b> Models E102/F102	A weakened header bond can result in one or more of the following device behaviors: <ul style="list-style-type: none"><li>– Significant changes in measured lead impedance</li><li>– Noise on real-time or stored electrograms</li><li>– Intermittent inhibition of pacing</li><li>– Inappropriate anti-tachy pacing or shock therapy</li><li>– Loss of pacing therapy</li><li>– Loss of anti-tachy pacing and shock therapy</li></ul>
<b>TELIGEN DR</b> Models E110/E111/F110/F111	No patient deaths related to this behavior have been reported. Patients have required early device replacement due to inappropriate shocks and/or noise induced by pocket manipulation or arm movement.
<a href="#">Subpectoral Implant 2009 Physician Letter, Dec 01, 2009</a>	<i>Rate of Occurrence</i> The implant orientation of devices is not reported to Boston Scientific, making it difficult to provide rate of occurrence and prediction information. Two (2) reports have been received worldwide of subpectoral implants with weakened header bonds. An estimated 5% of approximately 77,000 COGNIS and TELIGEN devices worldwide have been implanted in a subpectoral location.
<a href="#">Subpectoral Implant 2009 Patient Letter, Dec 01, 2009</a>	The following factors may also impact the risk of failure if implanted in a subpectoral location: <ul style="list-style-type: none"><li>– Exact location of the patient’s ribs relative to the device</li><li>– Body size and/or muscle mass of the patient (risk may increase for larger/muscular patients)</li><li>– Activity level and/or occupation of the patient (risk may increase for more active patients)</li></ul>
	CURRENT STATUS 02-Jul-24
	<i>Reported events (worldwide)</i>  106 reports have been received worldwide of subpectoral implants with weakened header bonds. An estimated 10% of approximately 104,000 COGNIS and TELIGEN devices worldwide have been implanted in a subpectoral location.  There have been no reported patient deaths associated with this advisory.
	CURRENT RECOMMENDATION 02-Jul-24
	If a patient’s device was implanted subcutaneously, it is excluded from this advisory and no change to current patient management is recommended.  <b>For affected devices implanted in a subpectoral location:</b> <ul style="list-style-type: none"><li>– Follow patient at least once every three months as recommended in device instructions for use.</li><li>– Consider advising patients to contact their physician or clinic if they receive shocks, in order to ensure timely review of associated electrograms and other device data via in-clinic or remote interrogation.</li><li>– Where available, consider using the LATITUDE® Patient Management System to facilitate remote device checks between in-clinic follow-ups.</li></ul>
	Standard Warranty program available, please contact your local representative for terms and conditions.

# Trademarks

The following are trademarks of Boston Scientific Corporation, CRM Division (doing business as Cardiac Pacemakers, Inc., a Boston Scientific Company) used in connection with the goods or services indicated:

ACCOLADE	EQUIO	LUX-DX
ACUITY	ENDOTAK ENDURANCE	MOMENTUM
ACUITY X4	ENDOTAK ENDURANCE EZ	ORIGEN
ADVANTIO	ENDOTAK ENDURANCE RX	PERCIVA
ALTITUDE	ENDOTAK RELIANCE	PROPONENT
ALTRUA	ENERGEN	PUNCTUA
AUTOGEN	ESSENTIO	RELIANCE 4-FRONT
AVT	FINELINE	RESONATE
CHARISMA	FLEXTEND	SELUTE
COGNIS	FORMIO	SWEET PICOTIP
CONFIENT	INSIGNIA	SWEET TIP
CONTAK	INGENIO	TELIGEN
CONTAK RENEWAL	INGEVITY	VIGILANT
CONTAK RENEWAL TR	INCEPTA	VISIONIST
DYNAGEN	INLIVEN	VITALIO
EASYTRAK	INOGEN	VITALITY
EMBLEM	INTUA	4-SITE
ENDOTAK	INVIVE	

The following marks are registered trademarks for Intermedics, Inc and Cameron Health, Inc. (doing business as Cardiac Pacemakers, Inc., a Boston Scientific Company) used in connection with the goods or services indicated:

Q-TRAK	SQ-RX	S-ICD
--------	-------	-------



**Rhythm Management**

300 Boston Scientific Way  
Marlborough, MA 01752-1234  
**[www.bostonscientific.com](http://www.bostonscientific.com)**

*Medical Professionals:*  
*1.800.CARDIAC (227.3422)*  
*Patients and Families:*  
*1.866.484.3268*

© 2021 Boston Scientific Corporation  
or its affiliates. All rights reserved.

CRM-373910-AD