




# Furlow

## Disposable Insertion Tool

The Furlow Disposable Insertion Tool is designed to keep your operating theatre on track with unmatched control and reduced risks.<sup>1-5</sup>

A next-generation device that builds upon the proven legacy of the reusable Furlow Insertion Tool, the Furlow Disposable Insertion Tool delivers improved ergonomics, packaged sterility, and immediate availability.<sup>5</sup>

### Consistent performance EVERY TIME

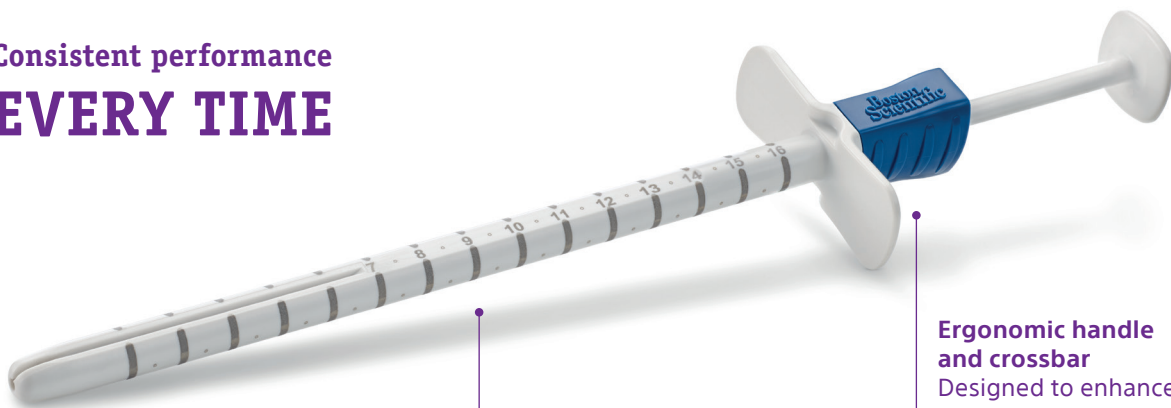

**Smooth shaft with tapered distal tip**  
Designed to streamline insertion<sup>5</sup>

**High-contrast, circumferential markings with new ½ cm indicators**  
Designed to increase visibility<sup>5</sup>

**Ergonomic handle and crossbar**  
Designed to enhance control<sup>5</sup>

**Locking obturator with haptic feedback**  
Designed to prevent unintentional separation and provide confirmation for needle loading and deployment<sup>5</sup>

### Designed to reduce the risk of contamination<sup>1-5</sup>

Sterilized during manufacturing, the Furlow Disposable Insertion Tool is designed to remove the potential for improper reprocessing or incomplete sterilization, reducing the risk of contamination-related infection.<sup>1-5</sup> Paired with the Furlow Disposable Insertion Tool, our AMS 700™ Inflatable Penile Prosthesis with InhibiZone™ Antibiotic Surface Treatment is designed to give you greater confidence.<sup>5-9</sup> The new Furlow Disposable Insertion Tool is designed to help protect patients – and your hospital too. According to a US-based publication, an infected IPP may necessitate a replacement of the implant<sup>10</sup>, which in the context of the NHS England would equate to an economic burden of £10,163 per case (NHS England National Tariff Code LB74Z) or around €11,725 (OANDA Currency Converter as of 06.11.2023).<sup>11</sup>

### Ordering information

SAP material number/UPN	SAP material description	QTY per box	GTIN assigned	SAP material type
M00635400020	Furlow Disposable Insertion Tool	1 Each	00191506022181	ZOEM

1. Reprocessing of reusable medical devices. FDA. <https://www.fda.gov/medical-devices/products-and-medical-procedures/reprocessing-reusable-medical-devices>. Accessed May 4, 2023.

2. Dancer SJ, Stewart M, Coulombe C, Gregori A, Viridi M. Surgical site infections linked to contaminated surgical instruments. *J Hosp Infect.* 2012;81:231-238.

3. Yafi FA, Furr J, El-Khatib FM, et al. Prospective analysis of cultures from the Furlow insertion tool: a possible etiology for penile prosthesis infections. *Int J Impot Res.* 2021;33:291-295.

4. Gross MS. Comment on Prospective analysis of cultures from the furlow insertion tool: a possible etiology for penile prosthesis infections. *Int J Impot Res.* 2021;33:382.

5. Data on file with Boston Scientific.

6. Carson CC III, Mulcahy JJ, Harsh MR. Long-term infection outcomes after original antibiotic impregnated inflatable penile prosthesis implants: up to 7.7 years of follow-up. *J Urol.* 2011 Feb;185(2):614-8.

7. Mulcahy JJ, Carson CC III. Long-term infection rates in diabetic patients implanted with antibiotic-impregnated versus nonimpregnated inflatable penile prostheses: 7-year outcomes. *Eur Urol.* 2011 Jul;60(1):167-72.

8. Nehra A, Carson CC III, Chapin AK, et al. Long-term infection outcomes of a 3-piece antibiotic impregnated penile prostheses used in replacement implant surgery. *J Urol.* 2012 Sep;188(3):899-903.

9. Mansouri MD, Boone TB, Darouiche RO. Comparative assessment of antimicrobial activities of antibiotic-treated penile prostheses. *Eur Urol.* 2009 Dec;56(6):1039-45.

10. Darouiche RO. Treatment of infections associated with surgical implants. *N Engl J Med.* 2004;350:1422-1429.

11. NHSPS\_23-24 Prices Workbook