




Furlow

Disposable Insertion Tool

The Furlow Disposable Insertion Tool is designed to keep your operating room on track with unmatched control and reduced risks.¹⁻⁵

A next-generation device that builds upon the proven legacy of the reusable Furlow Insertion Tool, the Furlow Disposable Insertion Tool delivers improved ergonomics, packaged sterility, and immediate availability.⁵

Consistent performance **EVERY TIME**

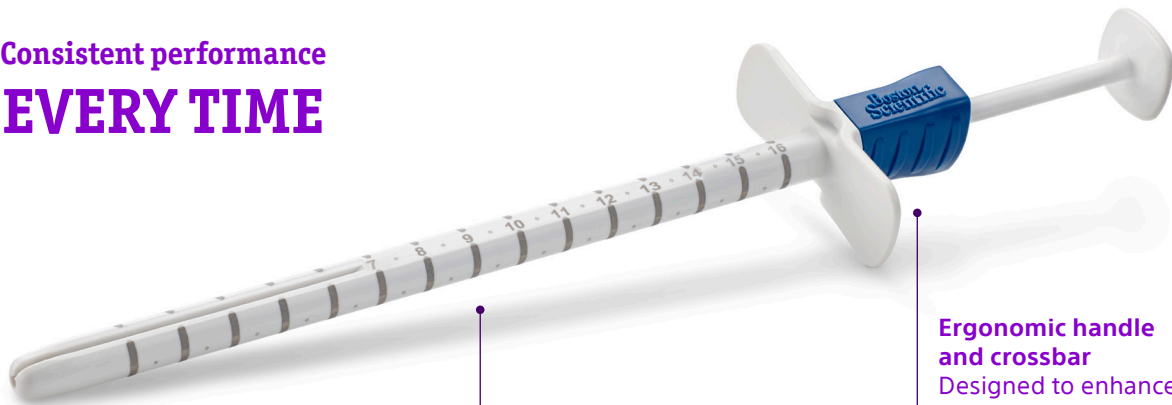

Smooth shaft with tapered distal tip
Designed to streamline insertion⁵

High-contrast, circumferential markings with new ½ cm indicators
Designed to increase visibility⁵

Ergonomic handle and crossbar
Designed to enhance control⁵

Locking obturator with haptic feedback
Designed to prevent unintentional separation and provide confirmation for needle loading and deployment⁵

Designed to reduce the risk of contamination¹⁻⁵

Sterilized during manufacturing, the Furlow Disposable Insertion Tool is designed to remove the potential for improper reprocessing or incomplete sterilization, reducing the risk of contamination-related infection.¹⁻⁵ Paired with the Furlow Disposable Insertion Tool, our AMS 700™ Inflatable Penile Prosthesis with InhibiZone™ Antibiotic Surface Treatment is designed to give your patients greater confidence. The new Furlow Disposable Insertion Tool is designed to help protect patients – and your hospital too, given a 2004 publication estimated the average cost of medical and surgical treatment for an infected IPP to be \$35,000.⁶

Ordering information

SAP material number/UPN	SAP material description	QTY per box	GTIN assigned	SAP material type
M00635400020	Furlow Disposable Insertion Tool	1 Each	00191506022181	ZOEM

1. Reprocessing of reusable medical devices. FDA. <https://www.fda.gov/medical-devices/products-and-medical-procedures/reprocessing-reusable-medical-devices>. Accessed May 4, 2023.
 2. Dancer SJ, Stewart M, Coulombe C, Gregori A, Virdi M. Surgical site infections linked to contaminated surgical instruments. *J Hosp Infect.* 2012;81:231-238.
 3. Yafi FA, Furr J, El-Khatib FM, et al. Prospective analysis of cultures from the Furlow insertion tool: a possible etiology for penile prosthesis infections. *Int J Impot Res.* 2021;33:291-295.
 4. Gross MS. Comment on Prospective analysis of cultures from the furlow insertion tool: a possible etiology for penile prosthesis infections. *Int J Impot Res.* 2021;33:382.
 5. Data on file with Boston Scientific.
 6. Darouiche RO. Treatment of infections associated with surgical implants. *N Engl J Med.* 2004;350:1422-1429.