



**Boston
Scientific**
Advancing science for life™

 | **Staying connected**




The myLUX™ Patient App transmits heart rhythm data stored on your LUX-Dx™ insertable cardiac monitor (ICM) device to your clinic. It is very important to keep the app connected so your health care provider can monitor your heart rhythm remotely. **Be sure to always follow these best practices.**



To learn more about the myLUX™ Patient App, scan this QR code to visit the myLUX™ patient website.


"LUX-Dx ICMs" includes LUX-Dx™, LUX-Dx II™ and LUX-Dx II+™ ICM Systems.

The downloadable myLUX™ Patient App and RhythmCARE™ Assist Service may be available for compatible LUX-Dx™ ICMs. Check with your health care provider for more information.



1

Keep the mobile device charged, powered on, and connected to the internet via cellular signal or Wi-Fi connection.



2

Keep Bluetooth® on so the app can connect to your ICM device.



3

Keep the mobile device within 6 feet (2 meters) of you while you're sleeping at night.




4


If you see a red screen and the exclamation point icon, the app is not connected. Tap **Check your connection**. Then follow the on-screen instructions.

A green screen appears when the app is successfully reconnected. Tap **Exit**.

iPhone

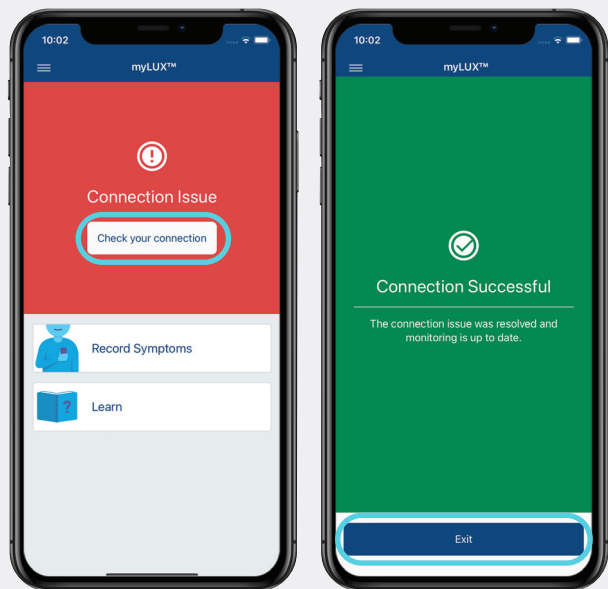

Android or Boston Scientific Provided Mobile Device

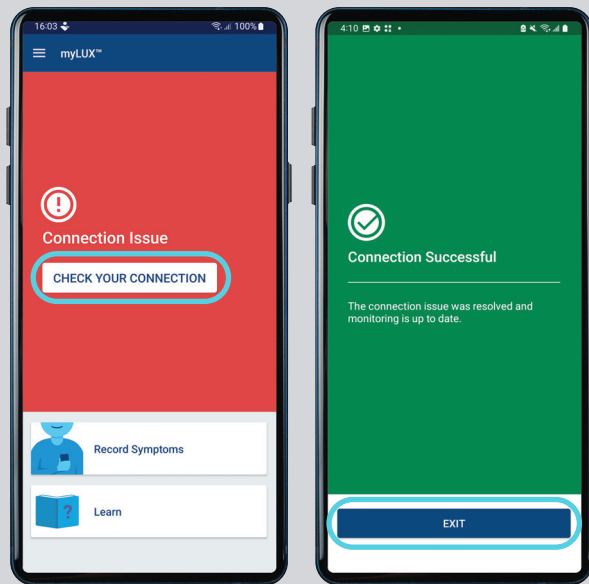


Some pictures of phone screens and buttons may look different on your mobile device, based on specific phone models or OS versions.




5

Open the myLUX™ Patient App often. Always look for a blue screen and a check mark icon after you open the app. This confirms that your monitoring is up to date. No further action is needed from you.

iPhone

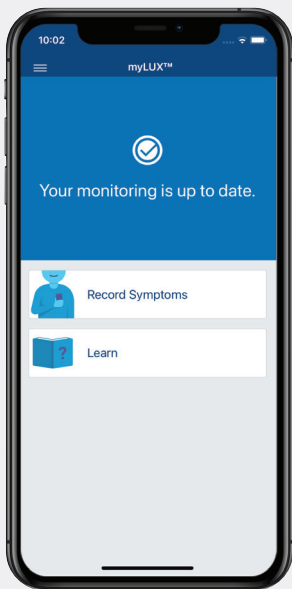

Android or Boston Scientific Provided Mobile Device

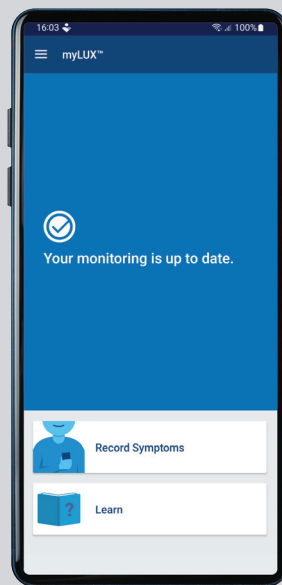


Some pictures of phone screens and buttons may look different on your mobile device, based on specific phone models or OS versions.



6


If you're utilizing the downloadable myLUX™ Patient App on your personal smartphone, remember these important things:

- **Do not quit** (i.e., do not swipe up to close the app) or **uninstall the app**.
- **If you restart your smartphone**, be sure to tap the app icon to **reopen** it.

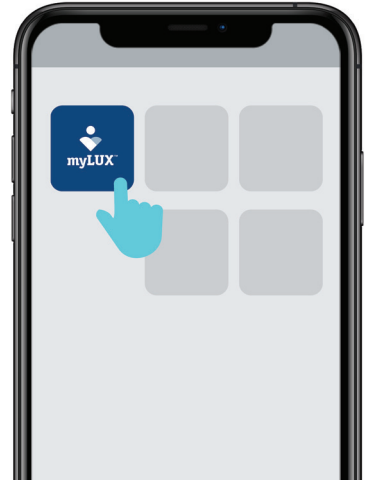


- Keep notifications turned on for the myLUX Patient App.

iPhone

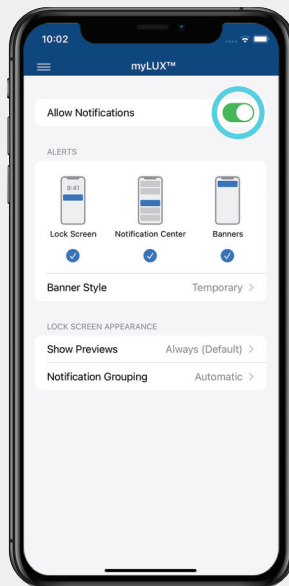


Android

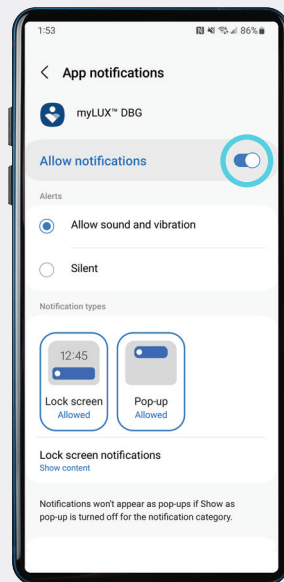


- Keep background refresh and background data usage on.

iPhone

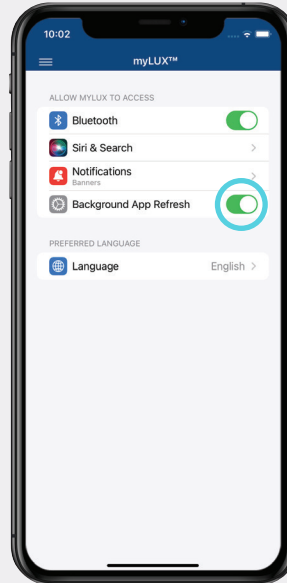


Android

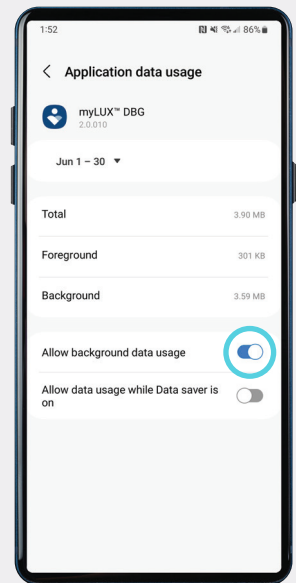


- Disable features that reduce the ability of the app to perform device checks in the background (e.g., power saving, low power, battery optimization, etc.).

iPhone

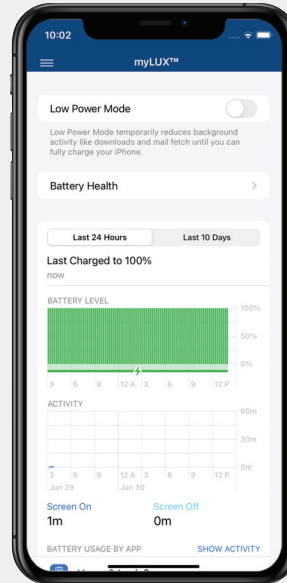

Android

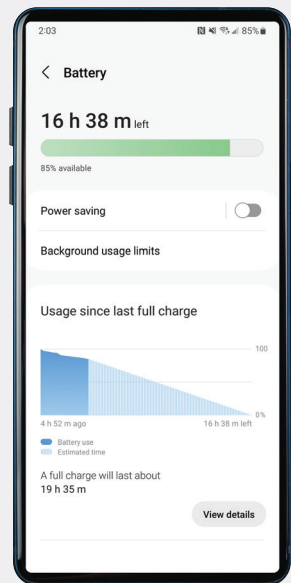

Need help?

Call Boston Scientific RhythmCARE™ Patient Services at **1-866-484-3268**, Monday–Friday during business hours, and select the option for LUX-Dx™ ICM.

If you need immediate medical attention, call your health care provider or seek emergency medical services.

myLUX™ Patient App and Insertable Cardiac Monitor System Important Information

The ICM system consists of the following: Insertable Cardiac Monitor ("ICM device"); Magnet; and myLUX patient app ("app"). The myLUX™ Patient App is for use with a BSC Insertable Cardiac Monitor (ICM) system which is a small device designed to monitor and record your heart rhythm once it has been placed under your skin. This information is shared via an automatic transmission to the clinic and your doctor for medical evaluation. The ICM and app are not intended to assist with medical emergencies; this means that it doesn't provide any treatment to the potential rhythms that could be recorded. Your myLUX™ Patient App is designed to work only with the ICM that your doctor has prescribed and implanted in you.

The ICM system does not treat cardiac arrhythmias (abnormal heartbeats that are too fast, too slow, or irregular), but rather it collects information for your health care provider to use to support their medical evaluation of your symptoms or condition. The ICM device's monitoring of your heart will not cause any noticeable sensations. Your ICM system is set up to automatically collect data stored on your ICM device and send it to your clinic to review according to the schedule your healthcare provider has set up. Your health care provider may also ask you to manually transmit data, however additional instruction will be provided if you need to do this as it should only be done on a limited basis.

Electromagnetic fields are created by devices which use electricity, including those which are plugged into a wall outlet or battery operated. Devices which emit strong electromagnetic fields may have the potential to temporarily interfere with your ICM device's ability to detect and monitor your heart rhythm. They could also delay or prolong communication between your ICM device and your myLUX™ Patient app.

The magnet when provided with the ICM system may cause interference with devices sensitive to magnetic fields such as hearing aids, pacemakers, and other implanted devices. It can also permanently disable some magnetic strip cards.

Ask your health care provider if you have questions about any risks with using the myLUX™ App, the magnet or your ICM device.

Please refer to the Patient Handbook for the full warnings, precautions and important safety information.

Rx only

92505919 C

All trademarks are the property of their respective owners.

Boston Scientific

Advancing science for life™

Cardiology

300 Boston Scientific Way
Marlborough, MA 01752-1234
www.bostonscientific.com

Medical Professionals:
1.800.CARDIAC (227.3422)
Patients and Families:
1.866.484.3268

© 2026 Boston Scientific Corporation
or its affiliates. All rights reserved.

CRM-1640507-AB Rx only.